

AperTO - Archivio Istituzionale Open Access dell'Università di Torino

Water and microbial monitoring technologies towards the near future space exploration

This is the author's manuscript

Original Citation:

Availability:

This version is available <http://hdl.handle.net/2318/1794956> since 2021-07-25T14:04:41Z

Published version:

DOI:10.1016/j.watres.2020.115787

Terms of use:

Open Access

Anyone can freely access the full text of works made available as "Open Access". Works made available under a Creative Commons license can be used according to the terms and conditions of said license. Use of all other works requires consent of the right holder (author or publisher) if not exempted from copyright protection by the applicable law.

(Article begins on next page)

1 **Water and microbial monitoring technologies towards the near future space exploration**

2

3 **Authors**

4 Stefano Amalfitano^{1*}, Caterina Levantesi¹, Diego Copetti², Fabrizio Stefani², Ilaria
5 Locantore³, Vincenzo Guarnieri³, Cesare Lobascio³, Francesca Bersani⁴, Donatella Giacosa⁴,
6 Emmanouil Detsis⁵, Simona Rossetti¹

7

8 **Institutions**

9 ¹ Water Research Institute – National Research Council of Italy (IRSA-CNR), Via Salaria
10 Km 29,300, 00015 Monterotondo, Roma, Italy

11 ² Water Research Institute – National Research Council of Italy (IRSA-CNR), Via del Mulino
12 19, 20861 Brugherio, Monza-Brianza, Italy

13 ³ Thales Alenia Space Italia SpA, Strada Antica di Collegno, 253 - 10146 Turin, Italy

14 ⁴ Centro Ricerche SMAT, Società Metropolitana Acque Torino S.p.A., C.so Unità d'Italia
15 235/3, 10127 Torino, Italy

16 ⁵ European Science Foundation, 1 quai Lezay Marnésia, BP 90015, 67080 Strasbourg Cedex,
17 France

18

19 * Corresponding author.

20 Tel.: +39 06 90672 854. Fax: +39 06 90672 787.

21 E-mail address: amalfitano@irsa.cnr.it

22

23 **Abstract**

24 Space exploration is demanding longer lasting human missions and water resupply from
25 Earth will become increasingly unrealistic. In a near future, the spacecraft water monitoring
26 systems will require technological advances to promptly identify and counteract contingent
27 events of waterborne microbial contamination, posing health risks to astronauts with lowered
28 immune responsiveness. The search for bio-analytical approaches, alternative to those applied
29 on Earth by cultivation-dependent methods, is pushed by the compelling need to limit waste
30 disposal and avoid microbial regrowth from analytical carryovers. Prospective technologies
31 will be selected only if first validated in a flight-like environment, by following basic
32 principles, advantages, and limitations beyond their current applications on Earth. Starting
33 from the water monitoring activities applied on the International Space Station, we provide a
34 critical overview of the nucleic acid amplification-based approaches (i.e., loop-mediated
35 isothermal amplification, quantitative PCR, and high-throughput sequencing) and early-
36 warning methods for total microbial load assessments (i.e., ATP-metry, flow cytometry),
37 already used at a high readiness level aboard crewed space vehicles. Our findings suggest that
38 the forthcoming space applications of mature technologies will be necessarily bounded by a
39 compromise between analytical performances (e.g., speed to results, identification depth,
40 reproducibility, multiparametricity) and detrimental technical requirements (e.g., reagent
41 usage, waste production, operator skills, crew time). As space exploration progresses toward
42 extended missions to Moon and Mars, miniaturized systems that also minimize crew
43 involvement in their end-to-end operation are likely applicable on the long-term and suitable
44 for the in-flight water and microbiological research.

45

46 **Keywords:**

47 International Space Station; space missions; biomonitoring; water biological contamination

48	Contents	
49	1 Introduction	3
50	2 Water recycle and microbial monitoring aboard the International Space Station	5
51	2.1 The ISS water cycle	5
52	2.2 On-board water monitoring and microbial contamination.....	7
53	3 Nucleic acid amplification-based methods for microbial identification in space waters....	10
54	3.1 Sample pre-treatments and nucleic acid extraction in space.....	10
55	3.2 Target-based techniques for detection and quantification of nucleic acids	12
56	3.3 Sequencing-based “-omics” approaches for microbial community characterization ..	15
57	4 Real-time technologies for early warning microbial monitoring.....	18
58	4.1 ATP-metry	19
59	4.2 Flow cytometry	21
60	5 Comparative analysis of space-relevant technological features.....	24
61	6 System miniaturization and future challenges	29
62	7 Conclusions	32
63	Acknowledgements.....	33
64	References.....	33

65

66 **1 Introduction**

67 Liquid water is essential for all known Earth-derived life forms living in space conditions,
68 including microbes (McKay, 2014). The on-going space exploration has not yet demonstrated
69 whether the presence of extra-terrestrial water could indicate itself the occurrence of
70 microbial life, but the prevailing paradigm is that living microorganisms necessitate temporal
71 and spatial proximity with aqueous solutions for their metabolism (Martín-Torres et al., 2015;
72 Merino et al., 2019; Stevenson et al., 2015). In turn, the microbial contamination cannot be
73 thoroughly eliminated from Earth’s waters but only controlled and attenuated on the long-
74 term time scale (Lopez et al., 2019; Rettberg et al., 2019). Since space exploration has been
75 demanding longer lasting missions, the analysis of waterborne microorganisms turned out of
76 utmost importance for future human spaceflights, planetary outposts, and life-support systems
77 (Horneck et al., 2010).

78 The prevention of crew infectious waterborne diseases is retained among the highest
79 priorities particularly for long duration missions (Ott et al., 2014), since emergency resupply
80 is unrealistic and recycled water could represent the only suitable source for the on-board
81 activities. Most of the aquatic microorganisms found aboard the International Space Station
82 (ISS) do not generally constitute a severe hazard for human health (Blaustein et al., 2019;
83 Checinska Sielaff et al., 2019; Sobisch et al., 2019). However, they may threat astronauts
84 with reduced immune response, mostly following the microgravity stress conditions (Garrett-
85 Bakelman et al., 2019; Ott et al., 2016). Other concerning issues arise from microbial
86 influences on spacecraft integrity and function, owing to the potential corrosion and
87 degradation of stainless steel and other materials associated with the electronic equipment
88 and life support systems (Horneck et al., 2010; Yang et al., 2018; Zea et al., 2018). Therefore,
89 there is an increasing interest to improve the spacecraft water monitoring systems to identify
90 and possibly counteract contingent events of microbial contamination (Van Houdt et al.,
91 2012; Yamaguchi et al., 2014).

92 The definition, identification, and test of the microbial monitoring approaches suitable for the
93 on-board water quality control are challenged by several technical constraints (e.g., material
94 safety compatibility, resistance to launch vibration) and a minimal availability for managing
95 excess power, storage, volume, mass, and crew time (Allen et al., 2018). Moreover, selected
96 devices and their supporting reagents must remain viable for years, while operating safely
97 and reliably in extreme conditions (e.g., in the absence of gravity). Technology flexibility is
98 also critical, since monitoring systems should be able to detect different microbial targets
99 (e.g., fungi, protists, prokaryotes, viruses) and to accept samples of various origin, spanning
100 from biomedical (e.g., blood, urine, saliva samples, routine chemistry, cell cultures) to water
101 and environmental samples (Nelson, 2011).

102 In the next years, the Chinese modular space station, built on the experience gained from its
103 precursors Tiangong-1 and Tiangong-2, will be placed and operating in the Low Earth orbit
104 (Gibney, 2019). The sustainable human exploration of the Moon is programmed in the
105 meanwhile (El-Jaby et al., 2019; Pittman et al., 2016), whereas the human missions to the
106 surface of Mars are envisioned before 2040 (ISECG, 2018). Therefore, it is hypothesized that
107 only prospective methodological applications at a high technology readiness level (i.e., at
108 least validated in a flight-like environment; Straub, 2015) will be selected by following their
109 basic principles and current uses in Earth and space-analogue settings.

110 A number of review papers has recently emphasized the need for high-throughput
111 technologies to timely monitor and achieve the stringent microbial quality requirements of
112 future crewed space habitats (De Middeleer et al., 2019; Karouia et al., 2017; Liu, 2017;
113 Moissl-Eichinger et al., 2016; Mora et al., 2016; Yamaguchi et al., 2014).

114 In this article, we narrow the focus on promising bio-analytic technologies for quality
115 assessments of waters in space, with the aim to explore advantages and limitations beyond
116 their current applications on Earth. Starting from the rigorous housekeeping program and the
117 consolidated results of water monitoring activity on the ISS (Duncan et al., 2008; Limero and
118 Wallace, 2017), we provide a critical overview of the microbial monitoring approaches,
119 based on flexible technologies for the identification of microbial components and a total
120 contamination assessment (total microbial burden) in waters circulating on crewed space
121 vehicles.

122

123 **2 Water recycle and microbial monitoring aboard the International Space Station**

124 **2.1 The ISS water cycle**

125 The water recycling system innovations required to support ISS activities have been listed
126 among the major benefits for humanity (Detsis and Detsis, 2013; NASA et al., 2019). The

127 ISS is provided with potable water from different suppliers, coordinated by the space
128 agencies of United States (National Aeronautics and Space Administration - NASA), Russia
129 (Russian Federal Space Agency - Roscosmos), Europe (European Space Agency - ESA), and
130 Japan (Japanese Aerospace Exploration Agency - JAXA) (Bruce et al., 2005; Van Houdt et
131 al., 2012). All the possible necessary precautions to prevent external contamination are
132 applied throughout water transferring and loading steps over the entire treatment period
133 before the liftoff of supply modules. For instance, the American and Russian waters are
134 produced in conditioned and limited-access areas and preparation facilities, with no risk of
135 accidental water quality modifications during the production process. At the research center
136 of the Italian Società Metropolitana Acque Torino (SMAT), purified waters for space travels
137 are also processed upon selecting well and spring waters that most closely meet the physical,
138 chemical, and bacteriological quality standards for astronauts (Lobascio et al., 2004).
139 Currently on ISS, waters for direct human consumption are regularly delivered and recovered
140 in order to guarantee approximately 4 L per person per day (Figure 1). A reserve of potable
141 water (up to approx. 2000 L) is stored in contingency containers to maintain ISS operations in
142 response to emergency scenarios (Carter et al., 2018). Although routinely monitored and kept
143 constant, the overall water mass balance represents a recurrent major challenge owing to the
144 various ISS water needs (Pickett et al., 2020).
145 Beside the on-demand crew consumption, on-board waters are distributed for different
146 purposes, comprising hygiene and cleaning practices, urinal flushing, oxygen generation via
147 electrolysis, life-support systems, and flexible water-based experimental activities (e.g.,
148 vegetable and food production systems, animal physiology and behavioral adaptation tests)
149 (Baiocco et al., 2018; Chatani et al., 2015; Massa et al., 2016; Niederwieser et al., 2018;
150 Ronca et al., 2019; Wolff et al., 2018). Wastewaters are continuously collected and recycled
151 at high efficiency level (Pickett et al., 2020). In the US segment, the Water Recovery and

152 Management System was reported to recuperate up to 85% from crew urine and flush water,
153 along with the water content from liquid wastes and humidity condensate from the cabin.
154 Various containers, reservoirs, tanks and bellows are also necessary to maintain water
155 pressure and circulation through the distribution network (Carter et al., 2018).
156 Since microbial growth is unavoidable in persistent stagnation zones and at varying residence
157 times along the water distribution network (Lautenschlager et al., 2010; Ling et al., 2018), the
158 pre- and in-flight addition of biocides is used for residual microbial control. Molecular iodine
159 is applied in the U.S. segment, while the ionic silver level is amended in Russian waters, both
160 at low concentrations (i.e., not detrimental for human health) (Artemyeva, 2016; Lobascio et
161 al., 2004). Moreover, high temperature in the catalytic reactor, multifiltration beds within the
162 Water Processor Assembly, UV-C LEDs within the CO₂ Concentration Assembly of the
163 Advanced Closed Loop System, and novel antimicrobial coatings on various ISS surfaces
164 were proven effective against potential microbial biomass growth (Bockstahler et al., 2017;
165 Carter et al., 2018; Perrin et al., 2018; Petala et al., 2020; Roman et al., 2006; Sobisch et al.,
166 2019). Finally, the ISS is maintained at pressure and oxygen levels very close to those at sea
167 level on Earth, with a cabin temperature of about 22°C and a relative humidity of about 60%,
168 in order to minimize detrimental growth of microbial biofilms on cabin surfaces (Pierson et
169 al., 2013).

170

171 **2.2 On-board water monitoring and microbial contamination**

172 The achievement and maintenance of water quality standards are evaluated by systematic
173 monitoring procedures (Limero and Wallace, 2017). Major water physical-chemical
174 parameters including conductivity, pH, total organic, total inorganic and total carbon, nitrate,
175 potassium, chloride and ammonium are monitored in-flight, together with iodine and silver
176 levels (Artemyeva, 2016). Moreover, a robust monitoring program was implemented to verify

177 that risks of microbial contamination were within acceptable limits in samples collected from
178 different sites of the Russian and US segments, respectively once every three months and
179 each month (Pierson et al., 2013; Van Houdt and Leys, 2012). Crewmembers use handheld
180 equipment to monitor ISS waters and humidity condensate from surfaces. Chemical and
181 biological samples are taken concurrently and at a frequency that may change due to real-
182 time flight necessities (Pierson et al., 2013).

183 Water samples can be processed on-board by cultivation-based methods using the US-
184 supplied Water Microbiology Kit for the quantification of total heterotrophic bacteria and
185 coliforms (Bruce et al., 2005). The maximum total number of aerobic heterotrophic viable
186 bacterial cells, counted as colony forming units on a rich agar medium, was internationally
187 defined according to the concentration levels that are achievable with the current prevention
188 and monitoring technologies available and applicable for space (i.e., HPC \leq 50 CFU/ml).

189 Microbial quality standards are also set for ISS internal surfaces, from which humidity
190 condensate is collected (maximum bacterial load = 10000 CFU/100 cm²; maximum fungal
191 load = 100 CFU/100 cm²) (Van Houdt and Leys, 2012). Along with the on-board monitoring
192 activities, archival water samples are regularly collected in teflon bags (Figure 1), preserved,
193 and returned to Earth approximately every three months for post-flight analyses (Limero and
194 Wallace, 2017).

195 The microbial contamination level was above the former acceptability limits several times
196 during previous in-flight monitoring surveys. Events of microbial biofilm growth within
197 space vehicles were mainly associated with the water layer covering internal surfaces and life
198 support systems (La Duc et al., 2004; Novikova et al., 2006; Roman et al., 2006). Thus,
199 waters collected from humidity condensate were retained among the major sources of
200 microbiological hazard for potable water quality deterioration (Horneck et al., 2010).

201



202

203 **Figure 1.** A water drop floating on the ISS (upper left). The Italian astronaut Samantha
204 Cristoforetti and the Russian cosmonaut Salizhan Sharipov showing the Teflon bag (upper
205 right), the water tank (lower left) and removal system (lower right), used for drinking
206 purposes and water storage on the ISS (Credits: ESA and NASA).

207

208 Several cultivable microbial isolates obtained from spaceflights were mainly affiliated to
209 Bacteria and Fungi (Bruce et al., 2005; Coil et al., 2016; Novikova et al., 2006). For the
210 purposes of this review, it is worth noting that the analysis of the microbial cultivable fraction
211 were likely to provide only a limited snapshot of the highly diverse community found on the
212 ISS by cultivation-independent methods (Checinska Sielaff et al., 2019; Coil et al., 2016; De
213 Mideleer et al., 2019; Ichijo et al., 2016; Lang et al., 2017; Mora et al., 2019; Morris et al.,
214 2012). Despite major advantages arise from target-specific isolation and characterization of
215 different types of waterborne microorganisms and pathogens in pure culture, a number of
216 technical and logistic disadvantages characterizes the space application of cultivation-based
217 methods. The microgravity conditions provide conflicting results on microbial growth and

218 virulence of opportunistic human pathogens (Morrison et al., 2017; Zhang et al., 2019), while
219 the analysis of archival samples generates a detrimental time gap for a flight-supportive result
220 interpretation (Huang et al., 2018; Novikova et al., 2006). HPC was proven to be also
221 affected by carbon sources in cultivation media, the incubation time, and the initial microbial
222 load level (Amalfitano et al., 2018b). Finally, the prompt development and requirement
223 update of alternate bio-analytical technologies for microbial monitoring during space
224 exploration is pushed fundamentally by the need to avoid microbial regrowth from analytical
225 wastes (Wong et al., 2017).

226

227 **3 Nucleic acid amplification-based methods for microbial identification in space** 228 **waters**

229 Methods based on nucleic acid amplification offer the advantage of specific and fast
230 detection, easy automatization and standardization. Many of the limitations of cultivation-
231 based techniques adopted for bacterial detection and water quality monitoring are
232 overwhelmed by largely reducing the time required for the microbial identification including
233 also viable but not cultivable bacteria and un-cultivable pathogens.

234

235 **3.1 Sample pre-treatments and nucleic acid extraction in space**

236 Sample pre-treatment and nucleic acid extraction are key starting points for most of the
237 molecular approaches and product developments dedicated to microbial water quality
238 monitoring. Nucleic acids extracted from water samples are amplified to specific markers.
239 The extraction and purification of nucleic acids rely on cell lysis and the selective binding of
240 cellular DNA and RNA to solid surfaces through filtration and column-based protocols.
241 A fast biomolecular analysis can be conducted in space settings with the in-line
242 implementation of optimized protocols for fast DNA and RNA extraction and sample

243 preparation for sequencing. Published studies reported new promising field-deployable
244 amplification devices and approaches for on board applications (Boguraev et al., 2017;
245 Montague et al., 2018) (Figure 2). Simplified, sample processing and DNA purification,
246 strategies have currently been tested aboard the International Space Station (ISS). The
247 Wetlab-2 project has already developed and tested on the ISS a Sample Preparation Module
248 (SPM) to lyse cells, and to provide high quality extraction of nucleic acids extract, by
249 circumventing operational issues related to microgravity, surface tension alteration, reduced
250 operational space and handling expertise (Parra et al., 2017).

251 Numerous commercialized kits for solid-phase extraction allow handy and rapid nucleic acid
252 purification procedures, in which potential contaminants are removed through sequential
253 washing steps based on centrifugation or DNA separation by paramagnetic beads (Tan and
254 Yiap, 2009). Methods for the direct PCR amplification without DNA extraction were also
255 developed (Williams et al., 2017). Recent papers reported simplified methods for nucleic acid
256 purification using filtration membranes and DNA amplification from the nucleic acid directly
257 on filters (Kaliyappan et al., 2012; Rodriguez et al., 2016). Notably, a cellulose-paper-based
258 dipstick was used to efficiently bind, wash, and elute purified nucleic acids from different
259 matrices without any pipetting or electrical equipment (Zou et al., 2017).

260 Nevertheless, a major bottleneck for the in-flight application of amplification based
261 approaches still lies on the need for time-consuming and waste-producing sample
262 concentration and DNA extraction (Girones et al., 2010). In particular, the method sensibility
263 is lowered when amplifying targets present at low levels over the total extracted DNA
264 (Brandt and Albertsen, 2018). Suboptimal DNA extraction and purification are known to
265 affect results of biomolecular analysis, mainly owing to uncomplete lysis of more resistant
266 bacterial populations and poor removal of DNA polymerase inhibitors (Albertsen et al., 2015;
267 Girones et al., 2010). DNA purification requires effective cell disruption, inactivation of

268 nucleases, and purification of DNA from contaminants that might interfere with the
269 amplification efficiency. Residual extracellular DNA could not be easily discriminated from
270 that of viable dangerous microorganisms, thus leading to an overestimation of risk for human
271 health (Girones et al., 2010). Moreover, waterborne substances can concentrate together with
272 DNA during sample processing and inhibit polymerase enzymes, thus influencing the
273 sensitivity and reliability of the PCR-based microbial detection. Overall, the relative accuracy
274 and precision (i.e., repeatability and reproducibility) of nucleic acid amplification based
275 methods are affected by sample type and pre-treatment methods (concentration and DNA
276 extraction), thus requiring to be evaluated across the whole sample processing (Hospodsky et
277 al., 2010; Kralik and Ricchi, 2017).

278

279 **3.2 Target-based techniques for detection and quantification of nucleic acids**

280 The polymerase chain reaction (PCR) is widely used for detecting genes and microorganisms
281 of health concern in water (Ramírez-Castillo et al., 2015). Among these target-based
282 detection approaches, the loop-mediated isothermal amplification (LAMP) of nucleic acids
283 was retained as a rapid and sensible option (Zhao et al., 2015), with minimal requirements for
284 the in-flight water quality monitoring and pathogen detection (Ott et al., 2014). The
285 amplification takes place at isothermal temperature (60-65°C) and positive reactions can be
286 visualised by naked eye (i.e., without post-amplification steps) following the increase of
287 sample turbidity or colour owing to the addition of fluorescent dyes (Notomi et al., 2015).
288 Being less sensible than PCR to inhibition and not significantly influenced by non-target
289 DNA, direct LAMP assays are currently used with good analytical performances (Etchebarne
290 et al., 2017; Samhan et al., 2017). Low amount of DNA can be amplified up to generating 10^9
291 copies within 1 h and producing as final amplification product a complex stem-loop DNA,
292 with several inverted repeats of the target and cauliflower-like structures. Commercial kits for

293 the rapid on-site detection of water pathogens are already available for terrestrial
294 applications, also comprising quantitative real-time LAMP, reverse transcription RT-LAMP,
295 *in situ* LAMP, and viable LAMP (Notomi et al., 2015). For the scopes of this review, it is
296 worth noting that a rapid method for detecting approximately 1 CFU/100 ml of *Legionella*
297 *pneumophila* in tap water was developed and efficiently applied on field in less than 2
298 working hours through a direct on-filter LAMP amplification with live/dead propidium
299 monoazide (PMA) differentiation (Samhan et al., 2017).

300 Among the target-based quantification approaches, the quantitative PCR (qPCR) represents a
301 popular technique for the in-flight water quality monitoring (Oubre et al., 2013). The
302 quantification of target sequences is based on the development of a fluorescent signal
303 proportional to the amount of amplified product obtained during the PCR thermal cycles.
304 Multiplex qPCR can be used for the simultaneous detection and quantification of multiple
305 pathogens, consistently reducing analytical time and costs (Ibekwe et al., 2002; LaGier et al.,
306 2004). With low detection limits (<400 cells per sample) and volume requirements (<100 µl
307 of sample), qPCR assays are routinely applied in monitoring plans for the detection and
308 quantification of waterborne pathogens (Girones et al., 2010; Ramírez-Castillo et al., 2015).
309 Good repeatability and reproducibility of qPCR outcomes were reported for gene targets of
310 fecal origin and a standardized workflow achieved consistent results, with low intra- and
311 inter-laboratory coefficients of variation (median CV = 0.1-3.3% and 1.9-7.1%, respectively)
312 (Ebentier et al., 2013; Orin et al., 2012). A large body of the scientific literature has
313 documented the development and use of qPCR for pathogenic viruses, bacteria, protozoa, and
314 fungi (Kralik and Ricchi, 2017; Ramírez-Castillo et al., 2015). Through a pre-treatment with
315 cell membrane impermeant DNA intercalating dyes, the so-called Viable qPCR was applied
316 for discriminating between viable (with intact membrane) and dead (with damaged
317 membrane) bacteria, allowing the quantification of water- and food-borne pathogens such as

318 *Campylobacter*, *E. coli* O157:H7, *Legionella pneumophila*, *Salmonella*, *Cryptosporidium*
319 (Banihashemi et al., 2012; Brescia et al., 2009; Delgado-Viscogliosi et al., 2009).

320 Given the versatile applications of the numerous available assays, both LAMP and qPCR
321 have been retained as suitable water monitoring methods for long-term exploration missions.
322 Owing to the high sensitivity, specificity, and simple post-amplification steps to detect the
323 amplified targets, LAMP was proposed by the Japanese Aerospace Exploration Agency as
324 alternative microbial contamination monitoring system for the ISS (Ott et al., 2014). For the
325 analysis of crew health related genetic modifications, qPCR technologies have been
326 successfully tested on-board the ISS within the projects Gene in Space and Wet-lab2, devoted
327 to definition of a robust, user-friendly nucleic acid extraction and sequencing approach
328 aboard ISS (Boguraev et al 2017; <https://www.genesinspace.org/>;
329 https://www.nasa.gov/mission_pages/station/research/experiments/1913.html;
330 <https://www.nasa.gov/ames/research/space-biosciences/wetlab-2>). Moreover, the RAZOR EX
331 PCR, launched on Space-X 9 (July 2016) within Water Monitoring Suite project will allow
332 performing direct PCR amplification from water samples.

333 In all current space applications, however, the selected target-based detection and
334 quantification approaches require the use of disposable materials and labour intense
335 protocols, which will inevitably reduce their long-term applicability in space conditions. The
336 general precautions used on Earth to limit contamination risks, including the most stringent
337 procedures applied in clean rooms (Rettberg et al., 2019), might also represent a limiting
338 practical issue in the small close spacecraft environment, since the high sensibility of PCR-
339 based detection increases the chance of amplifying carry over contamination, with the
340 consequent production of false positive results. This is crucial for LAMP owing to the limited
341 accessibility to degradation of DNA products, while a major limitation of qPCR is also the
342 occurrence of inhibitors that can be co-concentrated or extracted along with nucleic acids

343 from the target microorganisms (Gibson et al., 2012). The presence of qPCR inhibitors
344 introduces a number of problems, ranging from low amplification efficiency and reduced
345 assay sensitivity to complete reaction failure and false negative results (Radstrom et al.,
346 2008).

347

348 **3.3 Sequencing-based “-omics” approaches for microbial community characterization**

349 The High-Throughput Sequencing (HTS) encloses a popular suite of technologies,
350 methodological approaches, and data elaboration workflows used to characterize the
351 phylogenetic composition of the total microbial community in different aquatic matrices. The
352 taxonomic classification is based on the huge amount of sequences generated by either a
353 portion of the cellular nucleic acid content or the whole genome, through the so-called
354 amplicon and shotgun sequencing approaches, respectively (Peabody et al., 2015).

355 The amplicon analysis represents the extension of sequencing based methods of organisms’
356 classification, defined by specific protocols under the general name of “genetic” or
357 “molecular barcoding” (Hebert and Gregory, 2005), which is based on the information
358 carried by a single conventional marker, such as the 16S rRNA for microorganisms.

359 The shotgun sequencing consists in generating millions of DNA fragments of different
360 lengths from a starting pool of genomes. These fragments cover a quote of the original
361 genomes inversely proportional to the genome lengths, and taxonomic assignment may be
362 quantitative according to the proportion of fragments classified for each taxon. The amplified
363 products are sequenced, controlled for quality, and assembled in longer contigs. The obtained
364 sequences are classified at different taxonomic levels, according to the best match with a
365 reference sequence database and following different similarity criteria (Segata et al., 2012).

366 Currently, the most used sequencing platforms are characterized by different technical
367 principles and include Roche 454 GS-FLX (pyrosequencing), Illumina MiSeq and HiSeq

368 (reversible terminator sequencing by synthesis), Ion PGM (semiconductor based sequencing
369 by synthesis), and the nanopore GridION and MinION™ (Check Hayden, 2015; Clooney et
370 al., 2016; Ghanbari et al., 2015; Glenn, 2011).

371 Performance evaluation and standardization of HTS workflows are still limited for water
372 microbial community characterization. The DNA extraction procedures and primers sets were
373 reported to influence the assessment of the bacterial community composition in drinking
374 waters, with a generally effective representation of the core abundant taxa at total cell
375 abundance levels of 10^3 - 10^5 cells/ml (Brandt and Albertsen, 2018). Moreover, the method
376 sensitivity was detrimentally affected owing to the occurrence of contaminating bacteria in
377 extraction kits and laboratory reagents (Salter et al., 2014).

378 HTS-based technologies have been already tested under microgravity conditions and directly
379 on the ISS (Carr et al., 2020; Castro-Wallace et al., 2017; McIntyre et al., 2016). The most
380 suitable candidate technology to be transported and mounted on the ISS was the MinION
381 pocket-size device (Figure 2), which can provide rapid identification up to 300 kb with single
382 strand and 60 kb with double strands reads (Jain et al., 2016). The integrity and activity of
383 nanopores, in which DNA/RNA molecules pass through during base reading, were not
384 adversely affected by storage conditions, launch, cosmic radiations or handling in
385 microgravity, and reusability of flow cells was warranted. Specific indications to avoid air
386 bubbles interference at the nanopores were implemented (Castro-Wallace et al., 2017;
387 Rizzardi et al., 2016). Moreover, MinION performances in sequencing a mixture of genomic
388 DNA from a virus, a bacterium, and of mammal mtDNA, were comparable to those of
389 MinION, Illumina MiSeq and PacBio RSII run on ground. Accuracy respect to MiSeq and
390 RSII was slightly inferior (89% identity to the reference genome, respect to > 99%), but
391 sufficient for sequence analysis. Sequencing reads were successfully assigned to the correct
392 reference sequences in 90% of cases. Likely, with the novel improved versions of flow cells,

393 the molecular detection of aquatic microorganisms will improve notably (Kilianski et al.,
394 2015). Tests also demonstrated that real-time metagenomics analysis was also possible by
395 using a laptop device that can be integrated in the ISS hardware. Considering genomic data
396 analysis, one of the least demanding platforms has been tested successfully simulating flight
397 conditions and hardware availability onboard of the ISS, demonstrating its realistic
398 applicability even on a laptop base (Castro-Wallace et al., 2017). Provided the adaptation of
399 hardware and instruments to the spatial and logistic limitations onboard, both the shotgun and
400 amplicon approaches, can be considered as suitable tools for microbial community
401 characterization and pathogen detection on the ISS.

402 The amplicon approach requires straightforward PCR amplification protocols, downstream
403 bioinformatics, and database searches. Nevertheless, this technique is prone to fail to detect
404 unknown or highly divergent 16S rRNA gene sequences, which may be associated to novel
405 or previously undetected pathogens. Moreover, taxonomic assignment is highly sensitive to
406 the gene region selected as a marker and to the assignment method (Claesson et al., 2010; Liu
407 et al., 2008; Tremblay et al., 2015), while accuracy of quantification can be affected by
408 the variability in the number of gene copies shown by microbial taxon and even between
409 individual cells of the same species (Větrovský and Baldrian, 2013). Finally, a common
410 scientific view of suitable markers for viruses is still missing (Chakraborty et al., 2014).

411 In comparison to amplicon analysis, the shotgun sequencing offers a wide genome coverage
412 of organisms, allowing the detection of unknown contaminants and the possibility to screen
413 for both bacteria and viruses. In the field of water quality monitoring, the shotgun sequencing
414 was used, for instance, as the benchmark method to assess the occurrence of potential
415 multiple waterborne pathogens, novel indicators for human sewage contamination, and
416 microbial safety of drinking water in relation to the efficiency of reclamation treatments
417 (Chao et al., 2013; Lu et al., 2015; McLellan and Eren, 2014; Newton et al., 2015). Although

418 the possibility to obtain up to a few thousands of base pairs for each read improved the
419 microbial identification specificity, non-trivial disadvantages include the initial skimming of
420 the huge number of produced reads, their quality check and assemblage in contigs useful for
421 classification, which require high computational effort and time (Tan et al., 2015).
422



423
424 **Figure 2.** The NASA astronaut Peggy Whitson performing the Genes in Space investigation
425 on the ISS using the miniPCR and MinION. Credits: NASA
426

427 **4 Real-time technologies for early warning microbial monitoring**

428 The total contamination assessment (total microbial burden) through the accurate
429 quantification of microbial cell abundance and viability in waters circulating is a recognized
430 necessity on space crewed vehicles (Morris et al., 2012). Different early-warning real-time
431 methods that target parameters at the single-cell level (e.g., cellular biomolecules, membrane
432 integrity, enzyme activity, substrate uptake) have been developed for water monitoring, but
433 only few can efficiently operate in flight-like and space settings.

434

435 **4.1 ATP-metry**

436 An option for real-time monitoring of biological contamination in water samples is the
437 analysis of adenosine triphosphate (ATP) cell content. The analysis is carried out through the
438 chemical and/or enzymatic extraction of this molecule from microbial cells, followed by the
439 measurement of light emission derived when the dissolved ATP, in presence of magnesium,
440 reacts with the luciferine (substrate) - luciferase (enzyme) complex. The emitted light
441 intensity is linearly related to the ATP concentration, easily measurable using a luminometer,
442 and gives virtually instant information (within minutes) of the metabolically active microbial
443 population. This peculiarity makes it suitable as an early-warning approach for measuring
444 bacterial contamination and monitoring water treatment efficacy in near real-time (Hammes
445 et al., 2010). The method is robust, easy to perform, and suitable to detect both cultivable and
446 uncultivable cells, with better estimates of total active microorganisms compared to
447 heterotrophic plate counts. The concomitant use of traditional cultivation-based approaches
448 showed levels of cultivable cells order of magnitude lower than those estimated by ATP
449 (Siebel et al., 2008; Zhang et al., 2019).

450 The ATP analysis was performed on pre-flight and post-flight ISS water samples and
451 revealed a biological contamination ranging between 0 (drinking water) and 4.9×10^4 cells/ml
452 (humidity condensate) (Bacci et al., 2019; La Duc et al., 2004). Recently, the viable microbial
453 contamination on-board ISS was reliably monitored on surface samples by intracellular ATP
454 measurement (Perrin et al., 2018; Venkateswaran et al., 2003). ATP assays were also proven
455 effective in monitoring microbial contamination on surfaces from an inflated lunar/Mars
456 analogous habitat during long-term human occupation (Mayer et al., 2016). The total (ATP
457 content from both dead and live microbes) and viable microorganisms (intracellular ATP
458 content) were in the range of 10^5 - 10^6 relative luminescence unit (RLU)/m². These results
459 were in line with ATP data measured directly on-board within the experiment T2 carried out

460 during Euromir-95 mission (Guarnieri et al., 1997). Recently, the ATP-metry was selected for
461 the real-time monitoring of the biological contamination on board ISS within the H2020
462 European project BLOWYSE (Biocontamination integrated control of wet systems for space
463 exploration, <http://biowyse.eu>), aimed at developing a compact, automatic, and microgravity-
464 compatible on-board systems for the prevention, monitoring and control of microbial load in
465 waters and on wet surfaces (Figure 3). A humid area sampler was recently developed and
466 patented (ref. 102018000009137, dated 03/10/2018) (Detsis et al., 2018; Guarnieri et al.,
467 2019).

468 Today, commercial kits for quantitative ATP-metry are available to monitor the microbial
469 biomass level in water and to validate cleaning and disinfection procedures, with a wide
470 number of bulk and intracellular ATP measurements on microbial communities reported from
471 natural and engineered aquatic environments (Abushaban et al., 2019; Fillinger et al., 2019;
472 van der Wielen and van der Kooij, 2010; Vang et al., 2014). Although the apparent
473 advantages, major technical limitations are related to the low sensitivity and result
474 reproducibility at low cell concentration and sample volume (< 100 µl), along with the
475 susceptibility to environmental conditions (e.g., pH, temperature, occurrence of enzyme
476 inhibitors). Some drawbacks of the method are partly circumvented by using external and
477 internal standards and by operating under controlled reproducible settings. Therefore, the
478 correlation between intracellular ATP content and microbial cell counts will rely on a robust
479 cross-calibration with results from other reference methods (Amalfitano et al., 2018b;
480 Hammes et al., 2010). It has been calculated that the average ATP-per-cell content is
481 approximately 1.75×10^{-10} nmol/cell or 6.87×10^{-17} g ATP/cell (Zhang et al., 2019).
482 However, the amount of per-cell ATP can be significantly influenced by the phylogenetic
483 affiliation and the cellular physiological status, with diverse ATP-content reported between

484 either eukaryotic or prokaryotic cells from the same cultures (Bajerski et al., 2018; Yaginuma
485 et al., 2015).

486

487 **4.2 Flow cytometry**

488 Ubiquitously applied from the bio-medical research to environmental sciences, flow
489 cytometry (FCM) is considered an unparalleled high-throughput technology for single cell
490 analysis (Robinson and Roederer, 2015). This generic technology allows the measure (-
491 metry) of the optical properties of cells (cyto-) transported by a liquid sheath (flow).

492 Following sample intake, a pressurized laminar flow is generated and suspended particles are
493 individually forced to cross a light source excitation point for scanning and evaluation. Light
494 scatter and fluorescence signals (either with or without a secondary staining with fluorescent
495 dyes) are detected at the single-cell level and instantly converted into digital information to
496 be shown on multidimensional plots, along with real-time data analysis and statistics
497 (Shapiro, 2005).

498 Flow cytometry is included in the roadmaps of national space agencies worldwide and
499 deemed as a necessary technology for defining and monitoring spaceflight-associated
500 requirements since early 80's. Owing to the high versatility for diagnostic medicine (e.g.,
501 hematology, immunology, and physiology), this technology was so far retained as a prime
502 asset for health monitoring and clinical laboratory diagnostics for astronauts, in view of the
503 upcoming deep-space exploration missions (Crucian and Sams, 2012). A flow cytometry
504 platform was already successfully tested on-board the ISS to monitor and understand the
505 physiological adaptations of astronauts to microgravity (Dubeau-Laramée et al., 2014; Phipps
506 et al., 2014) (Figure 3). Advanced developments of the prototype were based on
507 commercialized flow cytometer with significant additional engineering modifications, mostly
508 aimed to generate laminar particle flow (distinct from the standard sheath fluid based

509 method), and to reduce the significant amount of liquid biohazardous waste and energy
510 operating requirements. The laminar flow within the flow chamber was found to be
511 dramatically altered by microgravity. In turn, the unavoidable elimination of the fluid
512 mechanical setting for particle hydrodynamic focusing was proven to significantly reduce
513 liquid waste and the total system operational load, in terms either of instrument size and
514 weight or energy consumption (Cohen et al., 2011; Crucian and Sams, 2005).

515 Notwithstanding the recent system design improvements, peripheral blood cells has been
516 retained as the only target for first studies in space environments (McMonigal and Crucian,
517 2015). Since a flow cytometer can provide support to a wide range of scientific applications
518 (e.g., biology, microbiology, and environmental science), it is needless to point out that a
519 spaceflight compatible machine could satisfy the unmet flight requirements for water
520 monitoring and treatment to complete future long-duration missions in closed healthy
521 environments.


522 The high sensitivity for scanning very small objects (i.e., from virus-like-particles to
523 prokaryotes, to pico- and micro-eukaryotes) and the wide detectable cell concentration range
524 (generally between 10^2 and 10^7 cells ml⁻¹ without concentrating or diluting the samples)
525 represent unmatched features of this technology for water monitoring. A broad suite of assays
526 is available for microbial quality assessments in natural and engineered aquatic ecosystems
527 (Amalfitano et al., 2014; Boi et al., 2016; Gasol and Morán, 2015; Van Nevel et al., 2017).

528 Successful applications are reported to provide early warning indications of unexpected water
529 contamination events through the rapid detection of a variety of microbiological threats,
530 including pathogenic and potentially toxic microorganisms (Vital et al., 2010; Weisse and
531 Bergkemper, 2018; Yang et al., 2010). Moreover, flow cytometric measurements are suitable
532 to evaluate the efficiency of various industrial microbial bioprocesses (e.g., food and
533 pharmaceutical preparations) (Díaz et al., 2010), and the performances of engineered systems

534 for water treatment (Besmer and Hammes, 2016; Safford and Bischel, 2019). Remarkably,
535 FCM was also useful to determine the presence of nonliving organic and inorganic
536 substances, including nano- and micro-sized particles, suspended solids, flocs and aggregates
537 of various origins (Aulenta et al., 2013; Casentini et al., 2016; Liu et al., 2016). On-going
538 instrumental developments for on-site applications are directed to install flow cytometers on
539 either mobile units (e.g., ships and vehicles) or fixed locations (e.g., treatment plants, marine
540 buoys, off-shore platforms), with the possibility for automatic programmable staining of
541 aquatic microorganisms and remote data transfer (Buyschaert et al., 2018; Pomati et al.,
542 2011; Thyssen et al., 2007).

543 Leaving aside the high costs of all sophisticated systems, the need for specially trained staff is
544 likely to represent a major drawback in the daily scheduled monitoring practices. Moreover,
545 the reproducibility of cytometric data was reported to be adversely affected by changing cell
546 staining protocols (e.g., fixatives, type of fluorescent dye), incubation conditions (e.g.,
547 temperature, time to analysis), instrumental settings (e.g., fluidic and signal amplification
548 systems), and the source water (e.g., from natural or engineered systems) (Nescerecka et al.,
549 2016; Prest et al., 2013). Further work is also required to establish user-independent strategies
550 for gating and data handling (Amalfitano et al., 2018a; Koch et al., 2014). One more specific
551 challenge is the lack of phylogenetic resolution. Despite the enumeration of targeted taxa may
552 rely on specific fluorescence staining procedures (Couradeau et al., 2019; Manti et al., 2011;
553 Neuenschwander et al., 2015), the cytometric information characterizing different
554 subpopulations of microbial cells is generally ataxonomic. A direct link between cytometric
555 fingerprinting and microbial diversity, assessed by 16S rRNA gene amplicon sequencing,
556 was demonstrated in recent studies (Props et al., 2017, 2016). However, the computational
557 workflows are convoluted and still under development (Rubbens et al., 2019).

558

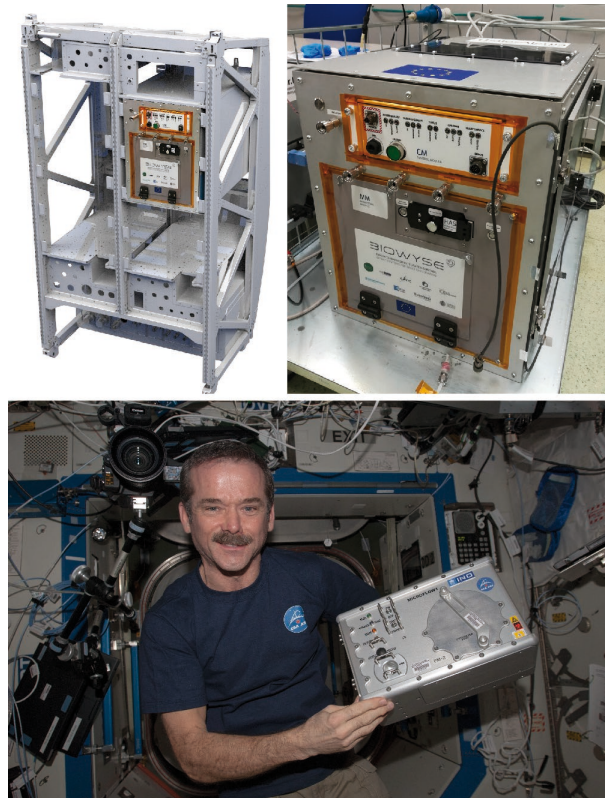

559


560 **Figure 3.** Integrated breadboard of the ATP-metry system, developed within the European
561 H2020 project BIOWYSE. The hardware was designed (upper left photo) and built (upper
562 right photo) to fly within the European Drawer Rack Mark 2. The photo below shows the
563 Canadian astronaut Chris Hadfield holding the flow cytometry platform Microflow1,
564 successfully deployed and tested on the ISS (Credits: BIOWYSE project consortium and
565 NASA).

566

567 **5 Comparative analysis of space-relevant technological features**

568 The procedural workflows of each of the mature technologies, herein entitled for water
569 microbial monitoring in space, comprise major steps and provide different types of results.

570 The overall time-to-results can vary from minutes to days, largely relying on user-dependent
571 manual operations and technological solutions for automation (figure 4).

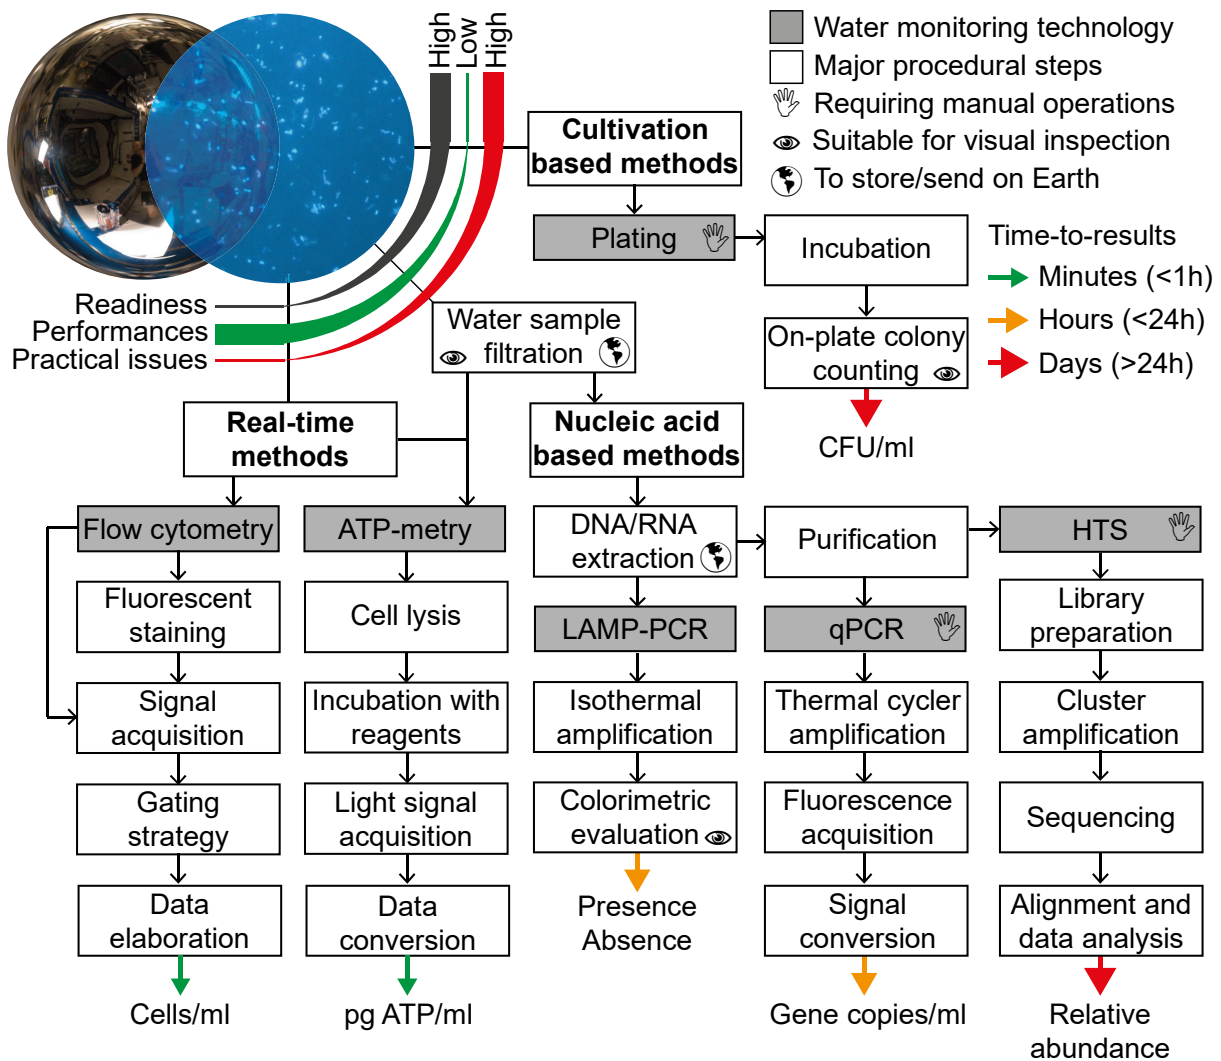

572

573 **Figure 4.** Workflows of mature technologies entitled for microbial water monitoring during
 574 space missions. Cultivation-, nucleic acid-based, and real-time methods are suitable to
 575 identify and quantify the waterborne microorganisms, ideally present in a drop of ISS water
 576 and visualized by epifluorescence microscopy on a filtration membrane (upper left pictures).
 577 Comparative levels of readiness, analytical performances, and practical issues were reported
 578 along with major procedural steps, timing, and types of achievable results.

579

580 Both current and future applications in space will be necessarily bounded by the definition of
 581 novel standards of microbial quality (i.e., other than those applied on Earth by cultivation-

582 dependent approaches) (Amalfitano et al., 2018b), but also by a compromise between the best
583 analytical performances and detrimental practical issues to cope with during spaceflights.
584 The implementation of successful on-board workflows will critically rely on the overall water
585 cycle management (Pickett et al., 2020), while fundamental analytical aspects can be
586 constrained by the minimal amount of water available for routine monitoring activities. For
587 example, technological accuracy and result reproducibility are directly linked to workable
588 water volumes and the constitutive occurrence of microbial targets in the sample (e.g.,
589 microbial cell abundance, per-cell gene copies, cell viability). Volumes required for accurate
590 and reproducible analyses will reasonably range between few tens of microliters (e.g., for
591 flow cytometric assessments) and hundreds of milliliters (e.g., for cultivation- and nucleic
592 acid-based methods), as also reported in terrestrial studies (Safford and Bischel, 2019).
593 Notably, sample filtration, a major pre-treatment step for ATP-metry and nucleic acid-based
594 methods, can selectively concentrate the microbial biomass and target microorganisms, while
595 minimizing the water loss for analytical needs. The filtering surfaces are also suitable for
596 visual inspection (e.g., by microscopy), storage, and comparative analysis (e.g., on Earth).
597 However, filtration can influence the composition of the dissolved organic matter of the
598 permeate water, possibly triggering microbial regrowth in the downstream distribution
599 system (Park et al., 2018), and it will also necessitate additional crew time for manual
600 operations (e.g., filter substitution, regeneration, disposal).
601 Sufficient data are not yet available from real space conditions to implement protocol details
602 within the procedural workflows. Although the selected technologies were demonstratively
603 applied under either simulated or real microgravity conditions, their own critical advantages
604 and limitations will require full reconsideration for flight-like and space applications.
605 From the one hand, analytical benefits will necessarily include the time needed to achieve
606 results (i.e., speed to results), the accuracy and flexibility in detecting specifically-selected

607 microbial targets (i.e., identification depth) with reproducible consistent results (i.e.,
608 reproducibility), and the number and multiple type of achievable results (i.e., herein named
609 multiparametricity). On the other hand, the operating conditions can be particularly stringent
610 and limiting the direct applicability in space, unless addressing critical requirements such as
611 reagent usage, waste production, operator skills, and crew time (table 1).

612 Using a simplistic pairwise comparison, we sought to emphasize that few selected
613 technological features have to be consciously retained from the methodological proof-of-
614 concept level up to the device deployment, instrumental demonstration, and routine use in the
615 on-board housekeeping program. Although the comparative scores were assigned
616 subjectively (table S1), it is likely evident that the stringent requirements of microbial water
617 monitoring in space cannot be met by a single technological solution.

618

619 **Table 1.** Advantages and limitations of the most promising approaches for microbial
620 monitoring in space settings. The selected technologies are flexible (i.e., applicable to
621 different microbial targets in samples of various origin), suitable for miniaturization and
622 automation with limited maintenance, and already tested in flight-like conditions. A
623 comparative score was arbitrarily assigned through a pairwise comparison matrix for each of
624 selected space-relevant technological features, including major analytical performances (i.e.,
625 speed to results, identification depth, reproducibility, multiparametricity – green marks) and
626 practical issues to cope with in space (i.e., reagent usage, waste production, operator skills,
627 crew time – red marks).

628

Technology	Advantages	Limitations	Analytical performances/ Practical issues	Comparative Scores	Applications in space		
Plate Cultivation	<ul style="list-style-type: none"> - No pretreatment - Detection limit 1 cell/100 ml - Low equipment requirements 	<ul style="list-style-type: none"> - No direct quantification - Risks of contamination - Reliant on cultivation conditions 	Speed to results	■ ■	La Duc et al., 2004		
			Identification depth	■ ■ ■ ■		Morrison et al., 2017	
			Reproducibility	■			Pierson et al., 2013
			Multiparametricity	■ ■			
			Reagent usage	■ ■ ■			
			Waste production	■ ■ ■ ■ ■ ■			
			Operator skills	■ ■ ■			
			Crew time	■ ■ ■ ■ ■			
LAMP	<ul style="list-style-type: none"> - Detection limit ~10² gene copies/ml - Unaffected by template conc. - No effects of inhibitory compounds 	<ul style="list-style-type: none"> - No direct quantification - Risks of contamination 	Speed to results	■ ■ ■ ■	Ott et al., 2014		
			Identification depth	■ ■ ■ ■ ■ ■			
			Reproducibility	■ ■ ■ ■			
			Multiparametricity	■ ■ ■			
			Reagent usage	■ ■ ■ ■			
			Waste production	■ ■ ■			
			Operator skills	■ ■			
			Crew time	■ ■			
qPCR	<ul style="list-style-type: none"> - Target-specific and quantitative - Detection limit ~10³ gene copies/ml 	<ul style="list-style-type: none"> - Pretreatment processing - Affected by template and inhibitory compounds - Reliant on PCR related issues 	Speed to results	■ ■ ■	Boguraev et al., 2017		
			Identification depth	■ ■ ■ ■ ■		Parra et al., 2017	
			Reproducibility	■ ■ ■			
			Multiparametricity	■ ■ ■ ■ ■			
			Reagent usage	■ ■ ■ ■ ■			
			Waste production	■ ■ ■ ■ ■			
			Operator skills	■ ■ ■ ■ ■			
			Crew time	■ ■ ■ ■ ■			
High Throughput Sequencing	<ul style="list-style-type: none"> - In-depth phylogenetic resolution - Specific for unknown non targeted microorganisms 	<ul style="list-style-type: none"> - Pretreatment processing - Reliant on PCR related issues - Complex data interpretation 	Speed to results	■ ■	Castro-Wallace et al., 2017		
			Identification depth	■ ■ ■		McIntyre et al., 2016	
			Reproducibility	■ ■			
			Multiparametricity	■ ■ ■ ■ ■ ■ ■			
			Reagent usage	■ ■ ■ ■ ■ ■ ■			
			Waste production	■ ■ ■ ■ ■ ■ ■			
			Operator skills	■ ■ ■ ■ ■ ■ ■			
			Crew time	■ ■ ■ ■ ■ ■ ■			
ATP-metry	<ul style="list-style-type: none"> - Real-time data (< 5 min) - Detection limit ~0.1 pg/ml 	<ul style="list-style-type: none"> - Unspecific detection - Destructive analysis - Risks of contamination 	Speed to results	■ ■ ■ ■ ■ ■ ■	Guarnieri et al., 1997		
			Identification depth	■		La Duc et al., 2004	
			Reproducibility	■ ■ ■ ■ ■			
			Multiparametricity	■			
			Reagent usage	■ ■			
			Waste production	■ ■			
			Operator skills	■			
			Crew time	■			
Flow cytometry	<ul style="list-style-type: none"> - No pretreatment - Quantitative and near-real time data (< 20 min) - Detection limit ~10² cells/ml 	<ul style="list-style-type: none"> - Complex data interpretation - Clogging issues 	Speed to results	■ ■ ■ ■ ■ ■	Dubeau-Laramée et al., 2014		
			Identification depth	■ ■		Phipps et al., 2014	
			Reproducibility	■ ■ ■ ■ ■ ■ ■			
			Multiparametricity	■ ■ ■ ■ ■			
			Reagent usage	■			
			Waste production	■			
			Operator skills	■ ■ ■ ■ ■ ■ ■			
			Crew time	■ ■ ■ ■ ■			

631 **6 System miniaturization and future challenges**

632 An important point is that the monitoring technologies can be mission-dependent, but only
633 those instruments that minimize crew involvement in their end-to-end operation are likely to
634 be applicable on the long-term (Karouia et al., 2017). Overall, the selected devices have to be
635 compact, suitable for automation, low power-consuming, and virtually invisible except when
636 needed (Limero and Wallace, 2017). The ground-based counterparts have already been
637 miniaturized using microfluidics, but the deployment of monitoring-effective tools onboard
638 spacecrafts will also require substantial reengineering and instrumental customization. The
639 instruments deployed so far have not been yet permanently used in spaceflight water
640 monitoring, yet numerous examples of successful international projects and commercial
641 partnerships dedicated to the human space exploration let argue that critical space water-
642 related tasks can be operatively accomplished at reasonable costs and times (< 5 years)
643 (Karouia et al., 2017).

644 Considerable progress has been made in miniature the onboard instrumentation to assess the
645 water microbiological contamination. This also includes microbial cultivation systems, such
646 as the AquaPad developed by the French CNES space agency (Augelli, 2018). The
647 microfluidic chips that allow cell isolation and incubation have been developed for ground-
648 based applications, and appear suitable for space uses. For example, the encapsulation of
649 single cells from a mixed microbial community into small droplet compartments of a water-
650 in-oil emulsion can offer further opportunities for physiological studies and viability assays
651 (e.g., metabolic by-products diffusion, resistance to toxicants, enzymatic activities) on clonal
652 populations isolated into plugs or micro-Petri dishes (Boedicker et al., 2008; Boitard et al.,
653 2015).

654 Considering the ability of microfluidic systems to efficiently conduct measurements on small
655 volumes of complex fluids without the need for a skilled operator, lab-on-a-chip technologies

656 and portable diagnostic devices have gained increased popularity for sensing a wide range of
657 water parameters and microbial pathogens even in the most remote settings (Mairhofer et al.,
658 2009). More recently, new qPCR platforms based on microfluidic technologies have been
659 developed allowing the simultaneous analysis of numerous genes and samples in volume
660 chambers of few nanoliters, placed at high density on a chip (Ricchi et al., 2017). Being less
661 sensitive to inhibitors than qPCR, the digital PCR (dPCR) is mainly applied to monitor gene
662 transcriptions in microbial cells without the need of a standard curve for gene copy
663 quantification (Devonshire et al., 2016).

664 The system miniaturization was also considered the most appealing trait for space
665 applications of the nanopore DNA sequencer MinION (Castro-Wallace et al., 2017). By
666 assembling miniaturized and lab-on-a-chip solutions, the Water Monitoring Suite developed
667 by NASA represents so far the best performing custom-built device applied successfully on
668 the ISS to monitor different water quality properties. Along with the HACH colorimeter and
669 the Organic Water Module, respectively used for inorganic and organic chemical
670 assessments, the hardware suite also includes the PCR-based instrument RAZOR EX, with
671 customized sample pouch kits containing all pre-loaded reagents necessary for sampling,
672 sample preparation, and real-time PCR

673 ([https://www.nasa.gov/mission_pages/station/research/experiments/explorer/Investigation.ht](https://www.nasa.gov/mission_pages/station/research/experiments/explorer/Investigation.html?id=1847)
674 [ml?id=1847](https://www.nasa.gov/mission_pages/station/research/experiments/explorer/Investigation.html?id=1847)). However, as space exploration progresses toward extended missions to cis-
675 lunar space and Mars, PCR-based and multi-omics instruments onboard spacecraft should not
676 be considered in separation from other technologies needed for the in-flight microbiological
677 research (Karouia et al., 2017).

678 In particular, microfluidic platforms developed for the direct cell detection showed promising
679 perspectives because of the potential for precise and easy-to-use analytical procedures. While
680 enhancing analytical performances, the system miniaturization presents also the advantages

681 of reduced consumption of reagents and the ability to integrate monitoring and isolation
682 procedures within a single device (Auroux et al., 2002). A simple microfluidic system was
683 successfully tested for rapid and semi-automated bacterial enumeration in freshwaters and
684 promising outcomes suggested its applicability to drinking waters under both ground and
685 space conditions (Yamaguchi et al., 2014). Moreover, both sensitivity and specificity of ATP-
686 metry and FCM can be also improved by miniaturizing the core systems down to scales
687 closer to the ones of microorganisms. A micro-fluorescence-activated cell sorting (μ FACS)
688 was used to sort out cells of interest by changing the flow direction after cell detection (Fu et
689 al., 1999). An integrated platform that combines two different force fields in a single
690 microfluidic device (Dielectrophoretic–Magnetic Activated Cell Sorter - iDMACS) was
691 applied for simultaneous sorting of multiple bacterial targets (Kim and Soh, 2009). More
692 recently, a high-throughput Raman flow cytometer was developed on a microfluidic chip for
693 the label-free molecular fingerprinting at the single-cell level (Hiramatsu et al., 2019).
694 The onboard laboratory miniaturization included also the fluidic components (e.g., pumps,
695 valves, electronics), thus paving the way to the use of advanced biosensors for screening food
696 safety and water quality in space (Roda et al., 2018). Following the proofs of concept and
697 wearable technologies suited to monitor astronauts' health, the biosensing diagnostic
698 instrumentation, most reasonably based on electrochemical and optical detectors, was argued
699 as a secondary future option for in-flight water biochemical analyses (Choi et al., 2018;
700 Limero and Wallace, 2017; Nelson, 2011). In particular, the amperometric biosensors were
701 proven sensitive to monitor different water analytes, chemical contaminants (e.g., pesticides,
702 organophosphates, carbamates), and numerous microbial biomarkers successfully targeted to
703 detect the major microbiological agents, food- and water-borne pathogens (e.g., *E. coli*,
704 *Salmonella*, *L. monocytogenes*, *C. jejuni*, *B. cereus*, *M. smegmatis*) (Grieshaber et al., 2008;
705 Velusamy et al., 2010). However, despite providing concrete benefits for health services and

706 our life on Earth and beyond, the spectroscopic and biosensing devices are still at a low level
707 of technological readiness for in-flight applications (García-Descalzo et al., 2019; Own et al.,
708 2019; Roda et al., 2018), thus falling out of the scopes of this review.

709 In general, a critical aspect of all microfluidic and lab-on-a-chip solutions is bound to the
710 very limited system reusability. Most miniaturized devices for terrestrial applications are of
711 single-use and, in many cases, based on disposable cartridges that cannot be safely stowed
712 onboard during long-term space missions. When cells are delivered to different system
713 compartments for collection, there is no clear approach for removal the analyzed samples
714 without compromising the system functioning and risking contamination. Clogging issues
715 may also interfere with the analyses due to the processing of large sample volumes. Reusable
716 systems have been tested, but their applications in space are likely constrained by the risk of
717 sample carryover, reduced analytical performance upon extended reuse, and the resources
718 required for cleaning and reactivation procedures. In this regard, the technological
719 development is highly demanding and still far from being accomplished in a near future.

720

721 **7 Conclusions**

- 722 • Current technologies for water microbial monitoring can satisfy the needs of long-term
723 space exploration missions at reasonable costs and times, although substantial
724 instrumental reengineering has to be considered.
- 725 • The suitable methodological applications at a high technology readiness level (i.e., at
726 least validated in a flight-like environment) will require reduced space to be allocated and
727 can potentially provide rapid and specific responses regarding the in-flight occurrence of
728 the microbiological contamination.
- 729 • The advanced biomolecular characterization of water samples from the ISS is promoting
730 a better understanding of the onboard levels and patterns of microbial contamination, thus

731 contributing to the development of space bound technologies for the rapid and specific
732 identification of microorganisms of health concerns.

- 733 • As space exploration progresses toward longer missions, PCR-based and multi-omics
734 approaches can be complemented by real-time technologies needed for the in-flight
735 microbiological research and suitable for the early-warning microbial monitoring of space
736 waters.

737

738 **Acknowledgements**

739 Authors wish to acknowledge H2020 Project called BIOWYSE “Biocontamination Integrated
740 cOntrol of Wet sYstems for Space Exploration” (<http://biowyse.eu>). Grant Agreement
741 number: 687447.

742

743 **References**

- 744 Abushaban, A., Salinas-Rodriguez, S.G., Mangal, M.N., Mondal, S., Goueli, S.A., Knezev,
745 A., Vrouwenvelder, J.S., Schippers, J.C., Kennedy, M.D., 2019. ATP measurement in
746 seawater reverse osmosis systems: Eliminating seawater matrix effects using a filtration-
747 based method. *Desalination* 453, 1–9. doi:10.1016/j.desal.2018.11.020
- 748 Albertsen, M., Karst, S.M., Ziegler, A.S., Kirkegaard, R.H., Nielsen, P.H., 2015. Back to
749 Basics – The Influence of DNA Extraction and Primer Choice on Phylogenetic Analysis
750 of Activated Sludge Communities. *PLoS One* 10, e0132783.
751 doi:10.1371/journal.pone.0132783
- 752 Allen, C.S., Giraud, M., Moratto, C., Yamaguchi, N., 2018. Spaceflight environment, in:
753 *Space Safety and Human Performance*. Elsevier, pp. 87–138. doi:10.1016/B978-0-08-
754 101869-9.00004-2
- 755 Amalfitano, S., Del Bon, A., Zoppini, A., Ghergo, S., Fazi, S., Parrone, D., Casella, P., Stano,

756 F., Preziosi, E., 2014. Groundwater geochemistry and microbial community structure in
757 the aquifer transition from volcanic to alluvial areas. *Water Res.* 65, 384–394.
758 doi:10.1016/j.watres.2014.08.004

759 Amalfitano, S., Fazi, S., Ejarque, E., Freixa, A., Romaní, A.M., Butturini, A., 2018a.
760 Deconvolution model to resolve cytometric microbial community patterns in flowing
761 waters. *Cytom. Part A* 93, 194–200. doi:10.1002/cyto.a.23304

762 Amalfitano, S., Levantesi, C., Garrelly, L., Giacosa, D., Bersani, F., Rossetti, S., 2018b.
763 Water Quality and Total Microbial Load: A Double-Threshold Identification Procedure
764 Intended for Space Applications. *Front. Microbiol.* 9, 1–10.
765 doi:10.3389/fmicb.2018.02903

766 Artemyeva, A.A., 2016. Analytical chemistry in water quality monitoring during manned
767 space missions. *Acta Astronaut.* 126, 11–17. doi:10.1016/j.actaastro.2016.04.016

768 Augelli, M., 2018. CADMOS: the French USOC. From a Quarter Century History to New
769 Prospects, in: 15th International Conference on Space Operations. American Institute of
770 Aeronautics and Astronautics, Reston, Virginia, pp. 1–11. doi:10.2514/6.2018-2519

771 Aulenta, F., Rossetti, S., Amalfitano, S., Majone, M., Tandoi, V., 2013. Conductive
772 magnetite nanoparticles accelerate the microbial reductive dechlorination of
773 trichloroethene by promoting interspecies electron transfer processes. *ChemSusChem* 6,
774 433–6. doi:10.1002/cssc.201200748

775 Auroux, P.-A., Iossifidis, D., Reyes, D.R., Manz, A., 2002. Micro Total Analysis Systems. 2.
776 Analytical Standard Operations and Applications. *Anal. Chem.* 74, 2637–2652.
777 doi:10.1021/ac020239t

778 Bacci, G., Amalfitano, S., Levantesi, C., Rossetti, S., Garrelly, L., Canganella, F., Bianconi,
779 G., Di Pilato, V., Rossolini, G.M., Mengoni, A., Fani, R., Perrin, E., 2019. Microbial
780 community composition of water samples stored inside the International Space Station.

781 Res. Microbiol. doi:10.1016/j.resmic.2019.04.003

782 Baiocco, G., Giraud, M., Bocchini, L., Barbieri, S., Locantore, I., Brussolo, E., Giacosa, D.,
783 Meucci, L., Steffenino, S., Ballario, A., Barresi, B., Barresi, R., Benassai, M.,
784 Ravagnolo, L., Narici, L., Rizzo, A., Carrubba, E., Carubia, F., Neri, G., Crisconio, M.,
785 Piccirillo, S., Valentini, G., Barbero, S., Giacci, M., Lobascio, C., Ottolenghi, A., 2018.
786 A water-filled garment to protect astronauts during interplanetary missions tested on
787 board the ISS. *Life Sci. Sp. Res.* 18, 1–11. doi:10.1016/j.lssr.2018.04.002

788 Bajerski, F., Stock, J., Hanf, B., Darienko, T., Heine-Dobbernack, E., Lorenz, M., Naujox, L.,
789 Keller, E.R.J., Schumacher, H.M., Friedl, T., Eberth, S., Mock, H.P., Kniemeyer, O.,
790 Overmann, J., 2018. ATP content and cell viability as indicators for cryostress across the
791 diversity of life. *Front. Physiol.* 9, 1–14. doi:10.3389/fphys.2018.00921

792 Banihashemi, A., Dyke, M.I., Huck, P.M., 2012. Long-amplicon propidium monoazide-PCR
793 enumeration assay to detect viable *Campylobacter* and *Salmonella*. *J. Appl. Microbiol.*
794 113, 863–873. doi:10.1111/j.1365-2672.2012.05382.x

795 Besmer, M.D., Hammes, F., 2016. Short-term microbial dynamics in a drinking water plant
796 treating groundwater with occasional high microbial loads. *Water Res.* 107, 11–18.
797 doi:10.1016/j.watres.2016.10.041

798 Blaustein, R.A., McFarland, A.G., Ben Maamar, S., Lopez, A., Castro-Wallace, S.,
799 Hartmann, E.M., 2019. Pangenomic Approach To Understanding Microbial Adaptations
800 within a Model Built Environment, the International Space Station, Relative to Human
801 Hosts and Soil. *mSystems* 4, 1–16. doi:10.1128/mSystems.00281-18

802 Bockstahler, K., Hartwich, R., Matthias, C.D., Laurini, D., Hovland, S., Witt, J., 2017. Status
803 of the Advanced Closed Loop System ACLS for Accommodation on the ISS. 47th
804 International Conference on Environmental Systems.

805 Boedicker, J.Q., Li, L., Kline, T.R., Ismagilov, R.F., 2008. Detecting bacteria and

806 determining their susceptibility to antibiotics by stochastic confinement in nanoliter
807 droplets using plug-based microfluidics. *Lab Chip* 8, 1265. doi:10.1039/b804911d

808 Boguraev, A.-S., Christensen, H.C., Bonneau, A.R., Pezza, J.A., Nichols, N.M., Giraldez,
809 A.J., Gray, M.M., Wagner, B.M., Aken, J.T., Foley, K.D., Copeland, D.S., Kraves, S.,
810 Alvarez Saavedra, E., 2017. Successful amplification of DNA aboard the International
811 Space Station. *npj Microgravity* 3, 26. doi:10.1038/s41526-017-0033-9

812 Boi, P., Amalfitano, S., Manti, A., Semprucci, F., Sisti, D., Rocchi, M.B., Balsamo, M., Papa,
813 S., 2016. Strategies for Water Quality Assessment: A Multiparametric Analysis of
814 Microbiological Changes in River Waters. *River Res. Appl.* 32, 490–500.
815 doi:10.1002/rra.2872

816 Boitard, L., Cottinet, D., Bremond, N., Baudry, J., Bibette, J., 2015. Growing microbes in
817 millifluidic droplets. *Eng. Life Sci.* 15, 318–326. doi:10.1002/elsc.201400089

818 Brandt, J., Albertsen, M., 2018. Investigation of Detection Limits and the Influence of DNA
819 Extraction and Primer Choice on the Observed Microbial Communities in Drinking
820 Water Samples Using 16S rRNA Gene Amplicon Sequencing. *Front. Microbiol.* 9, 1–
821 11. doi:10.3389/fmicb.2018.02140

822 Brescia, C.C., Griffin, S.M., Ware, M.W., Varughese, E.A., Egorov, A.I., Villegas, E.N.,
823 2009. Cryptosporidium Propidium Monoazide-PCR, a Molecular Biology-Based
824 Technique for Genotyping of Viable Cryptosporidium Oocysts. *Appl. Environ.*
825 *Microbiol.* 75, 6856–6863. doi:10.1128/AEM.00540-09

826 Bruce, R.J., Ott, C.M., Skuratov, V.M., Pierson, D.L., 2005. Microbial Surveillance of
827 Potable Water Sources of the International Space Station, in: SAE Technical Paper
828 Series. doi:10.4271/2005-01-2886

829 Buysschaert, B., Vermijs, L., Naka, A., Boon, N., De Gussemé, B., 2018. Online flow
830 cytometric monitoring of microbial water quality in a full-scale water treatment plant.

831 npj Clean Water 1, 16. doi:10.1038/s41545-018-0017-7

832 Carr, C.E., Bryan, N.C., Saboda, K.N., Bhattaru, S.A., Ruvkun, G., Zuber, M.T., 2020.

833 Nanopore Sequencing at Mars, Europa and Microgravity Conditions. bioRxiv.

834 doi:10.1101/2020.01.09.899716

835 Carter, L., Williamson, J., Brown, C.A., Bazley, J., Gazda, D., Schaezler, R., Thomas, F.,

836 2018. Status of ISS Water Management and Recovery, in: 48th International Conference

837 on Environmental Systems. American Institute of Aeronautics and Astronautics,

838 Albuquerque, NM; United States, pp. 1–16. doi:10.2514/6.2013-3509

839 Casentini, B., Falcione, F.T., Amalfitano, S., Fazi, S., Rossetti, S., 2016. Arsenic removal by

840 discontinuous ZVI two steps system for drinking water production at household scale.

841 Water Res. 106, 135–145. doi:10.1016/j.watres.2016.09.057

842 Castro-Wallace, S.L., Chiu, C.Y., John, K.K., Stahl, S.E., Rubins, K.H., McIntyre, A.B.R.,

843 Dworkin, J.P., Lupisella, M.L., Smith, D.J., Botkin, D.J., Stephenson, T.A., Juul, S.,

844 Turner, D.J., Izquierdo, F., Federman, S., Stryke, D., Somasekar, S., Alexander, N., Yu,

845 G., Mason, C.E., Burton, A.S., 2017. Nanopore DNA Sequencing and Genome

846 Assembly on the International Space Station. Sci. Rep. 7, 18022. doi:10.1038/s41598-

847 017-18364-0

848 Chakraborty, C., Doss, C.G.P., Patra, B.C., Bandyopadhyay, S., 2014. DNA barcoding to

849 map the microbial communities: current advances and future directions. Appl.

850 Microbiol. Biotechnol. 98, 3425–3436. doi:10.1007/s00253-014-5550-9

851 Chao, Y., Ma, L., Yang, Y., Ju, F., Zhang, X.X., Wu, W.M., Zhang, T., 2013. Metagenomic

852 analysis reveals significant changes of microbial compositions and protective functions

853 during drinking water treatment. Sci. Rep. doi:10.1038/srep03550

854 Chatani, M., Mantoku, A., Takeyama, K., Abduweli, D., Sugamori, Y., Aoki, K., Ohya, K.,

855 Suzuki, H., Uchida, S., Sakimura, T., Kono, Y., Tanigaki, F., Shirakawa, M., Takano,

856 Y., Kudo, A., 2015. Microgravity promotes osteoclast activity in medaka fish reared at
857 the international space station. *Sci. Rep.* 5, 14172. doi:10.1038/srep14172

858 Checinska Sielaff, A., Urbaniak, C., Mohan, G.B.M., Stepanov, V.G., Tran, Q., Wood, J.M.,
859 Minich, J., McDonald, D., Mayer, T., Knight, R., Karouia, F., Fox, G.E.,
860 Venkateswaran, K., 2019. Characterization of the total and viable bacterial and fungal
861 communities associated with the International Space Station surfaces. *Microbiome* 7, 50.
862 doi:10.1186/s40168-019-0666-x

863 Check Hayden, E., 2015. Pint-sized DNA sequencer impresses first users. *Nature* 521, 15–16.
864 doi:10.1038/521015a

865 Choi, J., Ghaffari, R., Baker, L.B., Rogers, J.A., 2018. Skin-interfaced systems for sweat
866 collection and analytics. *Sci. Adv.* 4, eaar3921. doi:10.1126/sciadv.aar3921

867 Claesson, M.J., Wang, Q., O’Sullivan, O., Greene-Diniz, R., Cole, J.R., Ross, R.P., O’Toole,
868 P.W., 2010. Comparison of two next-generation sequencing technologies for resolving
869 highly complex microbiota composition using tandem variable 16S rRNA gene regions.
870 *Nucleic Acids Res.* doi:10.1093/nar/gkq873

871 Clooney, A.G., Fouhy, F., Sleator, R.D., O’Driscoll, A., Stanton, C., Cotter, P.D., Claesson,
872 M.J., 2016. Comparing apples and oranges?: next generation sequencing and its impact
873 on microbiome analysis. *PLoS One* 11, e0148028.

874 Cohen, L.Y., Fortin, M., Leclair, S., Mermut, O., Dubeau-Laramee, G., 2011. Cellular and
875 molecular biology during spaceflight. *Gravitational Sp. Res.* 25, 60–62.

876 Coil, D.A., Neches, R.Y., Lang, J.M., Brown, W.E., Severance, M., Cavalier, D.D., Eisen,
877 J.A., 2016. Growth of 48 built environment bacterial isolates on board the International
878 Space Station (ISS). *PeerJ* 4, 1–11. doi:10.7287/peerj.preprints.1654v1

879 Couradeau, E., Sasse, J., Goudeau, D., Nath, N., Hazen, T.C., Bowen, B.P., Chakraborty, R.,
880 Malmstrom, R.R., Northen, T.R., 2019. Probing the active fraction of soil microbiomes

881 using BONCAT-FACS. *Nat. Commun.* 10, 2770. doi:10.1038/s41467-019-10542-0
882 Crucian, B., Sams, C., 2012. Flow cytometry methods to monitor immune dysregulation
883 associated with spaceflight, *Stress Challenges and Immunity in Space: From*
884 *Mechanisms to Monitoring and Preventive Strategies*. Springer Berlin Heidelberg,
885 Berlin, Heidelberg. doi:10.1007/978-3-642-22272-6
886 Crucian, B., Sams, C., 2005. Reduced Gravity Evaluation of Potential Spaceflight-
887 Compatible Flow Cytometer Technology. *Cytom. Part B* 9, 1–9.
888 doi:10.1002/cyto.b.20057
889 De Middeleer, G., Leys, N., Sas, B., De Saeger, S., 2019. Fungi and Mycotoxins in Space—A
890 Review. *Astrobiology* 19, ast.2018.1854. doi:10.1089/ast.2018.1854
891 Delgado-Viscogliosi, P., Solignac, L., Delattre, J.-M., 2009. Viability PCR, a Culture-
892 Independent Method for Rapid and Selective Quantification of Viable *Legionella*
893 *pneumophila* Cells in Environmental Water Samples. *Appl. Environ. Microbiol.* 75,
894 3502–3512. doi:10.1128/AEM.02878-08
895 Detsis, B., Detsis, E., 2013. The benefits brought by space—General public versus space
896 agencies perspectives. *Acta Astronaut.* 88, 129–137.
897 doi:10.1016/j.actaastro.2013.03.021
898 Detsis, E., Guarnieri, V., Lobascio, C., Saverino, A., Boscheri, G., Locantore, I., Garrelly, L.,
899 Simons, R., 2018. Biocontamination Integrated Control of Wet Systems for Space
900 Exploration (BIOWYSE).
901 Devonshire, A.S., O’Sullivan, D.M., Honeyborne, I., Jones, G., Karczmarczyk, M., Pavšič, J.,
902 Gutteridge, A., Milavec, M., Mendoza, P., Schimmel, H., Van Heuverswyn, F., Gorton,
903 R., Cirillo, D.M., Borroni, E., Harris, K., Barnard, M., Heydenrych, A., Ndusilo, N.,
904 Wallis, C.L., Pillay, K., Barry, T., Reddington, K., Richter, E., Mozioglu, E., Akyürek,
905 S., Yalçinkaya, B., Akgoz, M., Žel, J., Foy, C.A., McHugh, T.D., Huggett, J.F., 2016.

906 The use of digital PCR to improve the application of quantitative molecular diagnostic
907 methods for tuberculosis. *BMC Infect. Dis.* doi:10.1186/s12879-016-1696-7

908 Díaz, M., Herrero, M., García, L.A., Quirós, C., 2010. Application of flow cytometry to
909 industrial microbial bioprocesses. *Biochem. Eng. J.* 48, 385–407.
910 doi:10.1016/j.bej.2009.07.013

911 Dubeau-Laramée, G., Rivière, C., Jean, I., Mermut, O., Cohen, L.Y., 2014. Microflow1, a
912 sheathless fiber-optic flow cytometry biomedical platform: Demonstration onboard the
913 international space station. *Cytom. Part A* 85, 322–331. doi:10.1002/cyto.a.22427

914 Duncan, J.M., Bogomolov, V.V., Castrucci, F., Koike, Y., Comtois, J.M., Sargsyan, A.E.,
915 2008. Organization and management of the International Space Station (ISS)
916 multilateral medical operations. *Acta Astronaut.* 63, 1137–1147.
917 doi:10.1016/j.actaastro.2007.12.001

918 Ebentier, D.L., Hanley, K.T., Cao, Y., Badgley, B.D., Boehm, A.B., Ervin, J.S., Goodwin,
919 K.D., Gourmelon, M., Griffith, J.F., Holden, P.A., Kelty, C.A., Lozach, S., McGee, C.,
920 Peed, L.A., Raith, M., Ryu, H., Sadowsky, M.J., Scott, E.A., Domingo, J.S., Schriewer,
921 A., Sinigalliano, C.D., Shanks, O.C., Van De Werfhorst, L.C., Wang, D., Wuertz, S.,
922 Jay, J.A., 2013. Evaluation of the repeatability and reproducibility of a suite of qPCR-
923 based microbial source tracking methods. *Water Res.* 47, 6839–6848.
924 doi:10.1016/j.watres.2013.01.060

925 El-Jaby, S., Lewis, B.J., Tomi, L., 2019. On the decision making criteria for cis-lunar
926 reference mission scenarios. *Life Sci. Sp. Res.* 21, 25–39. doi:10.1016/j.lssr.2019.02.008

927 Etchebarne, B.E., Li, Z., Stedtfeld, R.D., Nicholas, M.C., Williams, M.R., Johnson, T.A.,
928 Stedtfeld, T.M., Kostic, T., Khalife, W.T., Tiedje, J.M., Hashsham, S.A., Hughes, M.J.,
929 2017. Evaluation of Nucleic Acid Isothermal Amplification Methods for Human
930 Clinical Microbial Infection Detection. *Front. Microbiol.* 8, 2211.

931 doi:10.3389/fmicb.2017.02211

932 Fillinger, L., Hug, K., Trimbach, A.M., Wang, H., Kellermann, C., Meyer, A., Bendinger, B.,
933 Griebler, C., 2019. The D-A-(C) index: A practical approach towards the
934 microbiological-ecological monitoring of groundwater ecosystems. *Water Res.* 163,
935 114902. doi:10.1016/j.watres.2019.114902

936 Fu, A.Y., Spence, C., Scherer, A., Arnold, F.H., Quake, S.R., 1999. A microfabricated
937 fluorescence-activated cell sorter. *Nat. Biotechnol.* doi:10.1038/15095

938 García-Descalzo, L., Parro, V., García-Villadangos, M., Cockell, C.S., Moissl-Eichinger, C.,
939 Perras, A., Rettberg, P., Beblo-Vranesevic, K., Bohmeier, M., Rabbow, E., Westall, F.,
940 Gaboyer, F., Amils, R., Malki, M., Marteinsson, V., Vannier, P., Ehrenfreund, P.,
941 Monaghan, E., Riedo, A., Cabezas, P., Walter, N., Gómez, F.G., 2019. Microbial
942 Markers Profile in Anaerobic Mars Analogue Environments Using the LDChip (Life
943 Detector Chip) Antibody Microarray Core of the SOLID (Signs of Life Detector)
944 Platform. *Microorganisms* 7, 365. doi:10.3390/microorganisms7090365

945 Garrett-Bakelman, F.E., Darshi, M., Green, S.J., Gur, R.C., Lin, L., Macias, B.R., McKenna,
946 M.J., Meydan, C., Mishra, T., Nasrini, J., Piening, B.D., Rizzardi, L.F., Sharma, K.,
947 Siamwala, J.H., Taylor, L., Vitaterna, M.H., Afkarian, M., Afshinnekoo, E., Ahadi, S.,
948 Ambati, A., Arya, M., Bezdán, D., Callahan, C.M., Chen, S., Choi, A.M.K., Chlipala,
949 G.E., Contrepois, K., Covington, M., Crucian, B.E., De Vivo, I., Dinges, D.F., Ebert,
950 D.J., Feinberg, J.I., Gandara, J.A., George, K.A., Goutsias, J., Grills, G.S., Hargens,
951 A.R., Heer, M., Hillary, R.P., Hoofnagle, A.N., Hook, V.Y.H., Jenkinson, G., Jiang, P.,
952 Keshavarzian, A., Laurie, S.S., Lee-McMullen, B., Lumpkins, S.B., MacKay, M.,
953 Maienschein-Cline, M.G., Melnick, A.M., Moore, T.M., Nakahira, K., Patel, H.H.,
954 Pietrzyk, R., Rao, V., Saito, R., Salins, D.N., Schilling, J.M., Sears, D.D., Sheridan,
955 C.K., Stenger, M.B., Tryggvadottir, R., Urban, A.E., Vaisar, T., Van Espen, B., Zhang,

956 J., Ziegler, M.G., Zwart, S.R., Charles, J.B., Kundrot, C.E., Scott, G.B.I., Bailey, S.M.,
957 Basner, M., Feinberg, A.P., Lee, S.M.C., Mason, C.E., Mignot, E., Rana, B.K., Smith,
958 S.M., Snyder, M.P., Turek, F.W., 2019. The NASA Twins Study: A multidimensional
959 analysis of a year-long human spaceflight. *Science* (80-.). 364.
960 doi:10.1126/science.aau8650

961 Gasol, J.M., Morán, X.A.G., 2015. Flow Cytometric Determination of Microbial Abundances
962 and Its Use to Obtain Indices of Community Structure and Relative Activity, in:
963 McGenity, T.J., Timmis, K.N., Nogales, B. (Eds.), *Hydrocarbon and Lipid Microbiology*
964 *Protocols: Single-Cell and Single-Molecule Methods*. Springer Berlin Heidelberg,
965 Berlin, Heidelberg, pp. 159–187. doi:10.1007/8623_2015_139

966 Ghanbari, M., Kneifel, W., Domig, K.J., 2015. A new view of the fish gut microbiome:
967 Advances from next-generation sequencing. *Aquaculture* 448, 464–475.
968 doi:10.1016/j.aquaculture.2015.06.033

969 Gibney, E., 2019. China reveals scientific experiments for its next space station. *Nature*.
970 doi:10.1038/d41586-019-01913-0

971 Gibson, K.E., Schwab, K.J., Spencer, S.K., Borchardt, M.A., 2012. Measuring and mitigating
972 inhibition during quantitative real time PCR analysis of viral nucleic acid extracts from
973 large-volume environmental water samples. *Water Res.*
974 doi:10.1016/j.watres.2012.04.030

975 Girones, R., Ferrús, M.A., Alonso, J.L., Rodriguez-Manzano, J., Calgua, B., de Abreu
976 Corrêa, A., Hundesa, A., Carratala, A., Bofill-Mas, S., 2010. Molecular detection of
977 pathogens in water - The pros and cons of molecular techniques. *Water Res.*
978 doi:10.1016/j.watres.2010.06.030

979 Glenn, T.C., 2011. Field guide to next-generation DNA sequencers. *Mol. Ecol. Resour.* 11,
980 759–769. doi:10.1111/j.1755-0998.2011.03024.x

- 981 Grieshaber, D., MacKenzie, R., Vörös, J., Reimhult, E., 2008. Electrochemical Biosensors -
982 Sensor Principles and Architectures. *Sensors* 8, 1400–1458. doi:10.3390/s80314000
- 983 Guarnieri, V., Gaia, E., Battocchio, L., Pitzurra, M., Savino, A., Pasquarella, C., Vago, T.,
984 Cotronei, V., 1997. New methods for microbial contamination monitoring: An
985 experiment on board the mir orbital station. *Acta Astronaut.* 40, 195–201.
986 doi:[https://doi.org/10.1016/S0094-5765\(97\)00102-1](https://doi.org/10.1016/S0094-5765(97)00102-1)
- 987 Guarnieri, V., Marchitelli, G., Boscheri, G., Locantore, I., 2019. Biocontamination Integrated
988 Control of Wet Systems for Space Exploration (BIOWYSE) – Test campaign results, in:
989 49th International Conference on Environmental Systems. Boston, Massachusetts, pp.
990 1–11.
- 991 Hammes, F., Goldschmidt, F., Vital, M., Wang, Y., Egli, T., 2010. Measurement and
992 interpretation of microbial adenosine tri-phosphate (ATP) in aquatic environments.
993 *Water Res.* 44, 3915–3923. doi:10.1016/j.watres.2010.04.015
- 994 Hebert, P.D.N., Gregory, T.R., 2005. The Promise of DNA Barcoding for Taxonomy. *Syst.*
995 *Biol.* 54, 852–859. doi:10.1080/10635150500354886
- 996 Hiramatsu, K., Ideguchi, T., Yonamine, Y., Lee, S., Luo, Y., Hashimoto, K., Ito, T., Hase,
997 M., Park, J.-W., Kasai, Y., Sakuma, S., Hayakawa, T., Arai, F., Hoshino, Y., Goda, K.,
998 2019. High-throughput label-free molecular fingerprinting flow cytometry. *Sci. Adv.* 5,
999 eaau0241. doi:10.1126/sciadv.aau0241
- 1000 Horneck, G., Klaus, D.M., Mancinelli, R.L., 2010. Space microbiology. *Microbiol Mol Biol*
1001 *Rev* 74. doi:10.1128/MMBR.00016-09
- 1002 Hospodsky, D., Yamamoto, N., Peccia, J., 2010. Accuracy, Precision, and Method Detection
1003 Limits of Quantitative PCR for Airborne Bacteria and Fungi. *Appl. Environ. Microbiol.*
1004 76, 7004–7012. doi:10.1128/AEM.01240-10
- 1005 Huang, B., Li, D.-G., Huang, Y., Liu, C.-T., 2018. Effects of spaceflight and simulated

1006 microgravity on microbial growth and secondary metabolism. *Mil. Med. Res.* 5, 18.
1007 doi:10.1186/s40779-018-0162-9

1008 Ibekwe, A.M., Watt, P.M., Grieve, C.M., Sharma, V.K., Lyons, S.R., 2002. Multiplex
1009 fluorogenic real-time PCR for detection and quantification of *Escherichia coli* O157:H7
1010 in dairy wastewater wetlands. *Appl. Environ. Microbiol.* doi:10.1128/AEM.68.10.4853-
1011 4862.2002

1012 Ichijo, T., Yamaguchi, N., Tanigaki, F., Shirakawa, M., Nasu, M., 2016. Four-year bacterial
1013 monitoring in the International Space Station—Japanese Experiment Module “Kibo”
1014 with culture-independent approach. *npj Microgravity* 2, 16007.
1015 doi:10.1038/npjmgrav.2016.7

1016 ISECG, 2018. The Global Exploration Roadmap, National Aeronautics and Space
1017 Administration. National Aeronautics and Space Administration, Washington, DC.

1018 Jain, M., Olsen, H.E., Paten, B., Akeson, M., 2016. The Oxford Nanopore MinION: delivery
1019 of nanopore sequencing to the genomics community. *Genome Biol.* 17, 239.
1020 doi:10.1186/s13059-016-1103-0

1021 Kaliyappan, K., Palanisamy, M., Govindarajan, R., Duraiyan, J., 2012. Microarray and its
1022 applications. *J. Pharm. Bioallied Sci.* 4, 310. doi:10.4103/0975-7406.100283

1023 Karouia, F., Peyvan, K., Pohorille, A., 2017. Toward biotechnology in space: High-
1024 throughput instruments for in situ biological research beyond Earth. *Biotechnol. Adv.*
1025 35, 905–932. doi:https://doi.org/10.1016/j.biotechadv.2017.04.003

1026 Kilianski, A., Haas, J.L., Corriveau, E.J., Liem, A.T., Willis, K.L., Kadavy, D.R.,
1027 Rosenzweig, C.N., Minot, S.S., 2015. Bacterial and viral identification and
1028 differentiation by amplicon sequencing on the MinION nanopore sequencer.
1029 *Gigascience* 4, 12. doi:10.1186/s13742-015-0051-z

1030 Kim, U., Soh, H.T., 2009. Simultaneous sorting of multiple bacterial targets using integrated

- 1031 Dielectrophoretic–Magnetic Activated Cell Sorter. *Lab Chip* 9, 2313.
1032 doi:10.1039/b903950c
- 1033 Koch, C., Harnisch, F., Schroeder, U., Müller, S., 2014. Cytometric fingerprints: Evaluation
1034 of new tools for analyzing microbial community dynamics. *Front. Microbiol.* 5, 1–12.
1035 doi:10.3389/fmicb.2014.00273
- 1036 Kralik, P., Ricchi, M., 2017. A Basic Guide to Real Time PCR in Microbial Diagnostics:
1037 Definitions, Parameters, and Everything. *Front. Microbiol.* 8.
1038 doi:10.3389/fmicb.2017.00108
- 1039 La Duc, M.T., Kern, R., Venkateswaran, K., 2004. Microbial monitoring of spacecraft and
1040 associated environments. *Microb. Ecol.* 47, 150–158.
- 1041 LaGier, M.J., Joseph, L.A., Passaretti, T. V., Musser, K.A., Cirino, N.M., 2004. A real-time
1042 multiplexed PCR assay for rapid detection and differentiation of *Campylobacter jejuni*
1043 and *Campylobacter coli*. *Mol. Cell. Probes.* doi:10.1016/j.mcp.2004.04.002
- 1044 Lang, J.M., Coil, D.A., Neches, R.Y., Brown, W.E., Cavalier, D., Severance, M., Hampton-
1045 Marcell, J.T., Gilbert, J.A., Eisen, J.A., 2017. A microbial survey of the International
1046 Space Station (ISS). *PeerJ* 5, e4029. doi:10.7717/peerj.4029
- 1047 Lautenschlager, K., Boon, N., Wang, Y., Egli, T., Hammes, F., 2010. Overnight stagnation of
1048 drinking water in household taps induces microbial growth and changes in community
1049 composition. *Water Res.* 44, 4868–4877. doi:10.1016/j.watres.2010.07.032
- 1050 Limero, T.F., Wallace, W.T., 2017. What Air and Water Quality Monitoring Is Needed to
1051 Protect Crew Health on Spacecraft? *New Sp.* 5, 67–78. doi:10.1089/space.2017.0004
- 1052 Ling, F., Whitaker, R., LeChevallier, M.W., Liu, W.-T., 2018. Drinking water microbiome
1053 assembly induced by water stagnation. *ISME J.* 12, 1520–1531. doi:10.1038/s41396-
1054 018-0101-5
- 1055 Liu, C., 2017. The theory and application of space microbiology: China’s experiences in

1056 space experiments and beyond. *Environ. Microbiol.* doi:10.1111/1462-2920.13472

1057 Liu, G., Ling, F.Q., van der Mark, E.J., Zhang, X.D., Knezev, A., Verberk, J.Q.J.C., van der
1058 Meer, W.G.J., Medema, G.J., Liu, W.T., van Dijk, J.C., 2016. Comparison of particle-
1059 associated bacteria from a drinking water treatment plant and distribution reservoirs with
1060 different water sources. *Sci. Rep.* 6, 20367. doi:10.1038/srep20367

1061 Liu, Z., DeSantis, T.Z., Andersen, G.L., Knight, R., 2008. Accurate taxonomy assignments
1062 from 16S rRNA sequences produced by highly parallel pyrosequencers. *Nucleic Acids*
1063 *Res.* 36, e120–e120. doi:10.1093/nar/gkn491

1064 Lobascio, C., Bruno, G., Grizzaffi, L., Meucci, L., Fungi, M., Giacosa, D., 2004. Quality of
1065 ATV Potable Water for ISS Crew Consumption, in: *SAE Technical Paper Series*. SAE
1066 International, pp. 1–10. doi:10.4271/2004-01-2491

1067 Lopez, J. V, Peixoto, R.S., Rosado, A.S., 2019. Inevitable future: space colonization beyond
1068 Earth with microbes first. *FEMS Microbiol. Ecol.* 95, 1–9. doi:10.1093/femsec/fiz127

1069 Lu, X., Zhang, X.X., Wang, Z., Huang, K., Wang, Y., Liang, W., Tan, Y., Liu, B., Tang, J.,
1070 2015. Bacterial pathogens and community composition in advanced sewage treatment
1071 systems revealed by metagenomics analysis based on high-throughput sequencing. *PLoS*
1072 *One.* doi:10.1371/journal.pone.0125549

1073 Mairhofer, J., Roppert, K., Ertl, P., 2009. Microfluidic Systems for Pathogen Sensing: A
1074 Review. *Sensors* 9, 4804–4823. doi:10.3390/s90604804

1075 Manti, A., Boi, P., Amalfitano, S., Puddu, A., Papa, S., 2011. Experimental improvements in
1076 combining CARD-FISH and flow cytometry for bacterial cell quantification. *J.*
1077 *Microbiol. Methods* 87, 309–315. doi:10.1016/j.mimet.2011.09.003

1078 Martín-Torres, F.J., Zorzano, M.-P., Valentín-Serrano, P., Harri, A.-M., Genzer, M.,
1079 Kempainen, O., Rivera-Valentin, E.G., Jun, I., Wray, J., Bo Madsen, M., Goetz, W.,
1080 McEwen, A.S., Hardgrove, C., Renno, N., Chevrier, V.F., Mischna, M., Navarro-

1081 González, R., Martínez-Frías, J., Conrad, P., McConnochie, T., Cockell, C., Berger, G.,
1082 R. Vasavada, A., Sumner, D., Vaniman, D., 2015. Transient liquid water and water
1083 activity at Gale crater on Mars. *Nat. Geosci.* 8, 357.

1084 Massa, G.D., Wheeler, R.M., Morrow, R.C., Levine, H.G., 2016. Growth chambers on the
1085 International Space Station for large plants. *Acta Horti.*
1086 doi:10.17660/ActaHortic.2016.1134.29

1087 McIntyre, A.B.R., Rizzardi, L., Yu, A.M., Alexander, N., Rosen, G.L., Botkin, D.J., Stahl,
1088 S.E., John, K.K., Castro-Wallace, S.L., McGrath, K., Burton, A.S., Feinberg, A.P.,
1089 Mason, C.E., 2016. Nanopore sequencing in microgravity. *npj Microgravity* 2, 16035.
1090 doi:10.1038/npjmgrav.2016.35

1091 McKay, C.P., 2014. Requirements and limits for life in the context of exoplanets. *Proc. Natl.*
1092 *Acad. Sci.* 111, 12628–12633. doi:10.1073/pnas.1304212111

1093 McLellan, S.L., Eren, A.M., 2014. Discovering new indicators of fecal pollution. *Trends*
1094 *Microbiol.* 22, 697–706. doi:10.1016/j.tim.2014.08.002

1095 McMonigal, K., Crucian, B., 2015. Health Monitoring and Clinical Laboratory Diagnostics
1096 for Astronauts. *Crit. Values* 7, 24–27. doi:10.1093/criticalvalues/7.4.24

1097 Merino, N., Aronson, H.S., Bojanova, D.P., Feyhl-Buska, J., Wong, M.L., Zhang, S.,
1098 Giovannelli, D., 2019. Living at the Extremes: Extremophiles and the Limits of Life in a
1099 Planetary Context. *Front. Microbiol.* 10. doi:10.3389/fmicb.2019.00780

1100 Moissl-Eichinger, C., Cockell, C., Rettberg, P., 2016. Venturing into new realms ?
1101 Microorganisms in space INTERNATIONAL SPACE STATION. *FEMS Microbiol.*
1102 *Rev.* 40, 722–737. doi:10.1093/femsre/fuw015

1103 Montague, T.G., Almansoori, A., Gleason, E.J., Copeland, D.S., Foley, K., Kraves, S.,
1104 Alvarez Saavedra, E., 2018. Gene expression studies using a miniaturized thermal cyclor
1105 system on board the International Space Station. *PLoS One* 13, e0205852.

1106 doi:10.1371/journal.pone.0205852

1107 Mora, M., Mahnert, A., Koskinen, K., Pausan, M.R., Oberauner-Wappis, L., Krause, R.,
1108 Perras, A.K., Gorkiewicz, G., Berg, G., Moissl-Eichinger, C., 2016. Microorganisms in
1109 confined habitats: Microbial monitoring and control of intensive care units, operating
1110 rooms, cleanrooms and the international space station. *Front. Microbiol.* 7, 1–20.
1111 doi:10.3389/fmicb.2016.01573

1112 Mora, M., Wink, L., Kögler, I., Mahnert, A., Rettberg, P., Schwendner, P., Demets, R.,
1113 Cockell, C., Alekhova, T., Klingl, A., Krause, R., Zolotariof, A., Alexandrova, A.,
1114 Moissl-Eichinger, C., 2019. Space Station conditions are selective but do not alter
1115 microbial characteristics relevant to human health. *Nat. Commun.* 10, 3990.
1116 doi:10.1038/s41467-019-11682-z

1117 Morris, H.C., Damon, M., Maule, J., Monaco, L.A., Wainwright, N., 2012. Rapid Culture-
1118 Independent Microbial Analysis Aboard the International Space Station (ISS) Stage
1119 Two: Quantifying Three Microbial Biomarkers. *Astrobiology* 12, 830–840.
1120 doi:10.1089/ast.2012.0863

1121 Morrison, M.D., Fajardo-Cavazos, P., Nicholson, W.L., 2017. Cultivation in space flight
1122 produces minimal alterations in the susceptibility of *Bacillus subtilis* cells to 72 different
1123 antibiotics and growth-inhibiting compounds. *Appl. Environ. Microbiol.* 83.
1124 doi:10.1128/AEM.01584-17

1125 NASA, CSA, ESA, JAXA, ROSCOSMOS, ASI, 2019. International Space Station Benefits
1126 for Humanity, 3rd ed. Houston.

1127 Nelson, E.S., 2011. Design principles for microfluidic biomedical diagnostics in space, in:
1128 Fazel, R. (Ed.), *Biomedical Engineering - From Theory to Applications*. InTech, Rijeka,
1129 Croatia, pp. 131–156. doi:10.5772/21669

1130 Nescerecka, A., Hammes, F., Juhna, T., 2016. A pipeline for developing and testing staining

1131 protocols for flow cytometry, demonstrated with SYBR Green I and propidium iodide
1132 viability staining. *J. Microbiol. Methods* 131, 172–180.
1133 doi:10.1016/j.mimet.2016.10.022

1134 Neuenschwander, S.M., Salcher, M.M., Pernthaler, J., 2015. Fluorescence in situ
1135 hybridization and sequential catalyzed reporter deposition (2C-FISH) for the flow
1136 cytometric sorting of freshwater ultramicrobacteria. *Front. Microbiol.* 6, 247.
1137 doi:10.3389/fmicb.2015.00247

1138 Newton, R.J., McLellan, S.L., Dila, D.K., Vineis, J.H., Morrison, H.G., Murat Eren, A.,
1139 Sogin, M.L., 2015. Sewage reflects the microbiomes of human populations. *MBio*.
1140 doi:10.1128/mBio.02574-14

1141 Niederwieser, T., Kociolek, P., Klaus, D., 2018. Spacecraft cabin environment effects on the
1142 growth and behavior of *Chlorella vulgaris* for life support applications. *Life Sci. Sp.*
1143 *Res.* 16, 8–17. doi:<https://doi.org/10.1016/j.lssr.2017.10.002>

1144 Notomi, T., Mori, Y., Tomita, N., Kanda, H., 2015. Loop-mediated isothermal amplification
1145 (LAMP): principle, features, and future prospects. *J. Microbiol.* 53, 1–5.
1146 doi:10.1007/s12275-015-4656-9

1147 Novikova, N., De Boever, P., Poddubko, S., Deshevaya, E., Polikarpov, N., Rakova, N.,
1148 Coninx, I., Mergeay, M., 2006. Survey of environmental biocontamination on board the
1149 International Space Station, in: *Research in Microbiology*. pp. 5–12.
1150 doi:10.1016/j.resmic.2005.07.010

1151 Orin, S., Mano, S., Lindsay, P., Catherine, K., Blackwood, A., Monica, G., Rachel, N.,
1152 Rebecca, B., Erin, S., Julie, K., Tamara, A., Christopher, Sinigalliano, David, W., John,
1153 G., Yiping, C., Steve, W., Harwood, V.J., Christopher, Staley, Kevin, O., Manju, V.,
1154 Richard, H., 2012. Correction to Interlaboratory Comparison of Real-Time PCR
1155 Protocols for Quantification of General Fecal Indicator Bacteria. *Environ. Sci. Technol.*

1156 46, 2478–2478. doi:10.1021/es300042b

1157 Ott, C.M., Marshburn, T., Nickerson, C.A., 2016. The International Space Station: an
1158 Extreme Environment for Key Host-Microbe Discoveries. *Microbe Mag.* 11, 253–261.
1159 doi:10.1128/microbe.11.253.1

1160 Ott, M., Pierson, D., Shirakawa, M., Tanigaki, F., Hida, M., Yamazaki, T., Shimazu, T.,
1161 Ishioka, N., 2014. Space Habitation and Microbiology: Status and Roadmap of Space
1162 Agencies. *Microbes Environ.* 29, 239–242. doi:10.1264/jsme2.ME2903rh

1163 Oubre, C.M., Birmele, M.N., Castro, V.A., Venkateswaran, K.J., Vaishampayan, P.A., Jones,
1164 K.U., Singhal, A., Johnston, A.S., Ozbolt, T.A., Jett, D.X., Roberts, M.S., Ott, M.,
1165 Roman, M.C., 2013. Microbial Monitoring of Common Opportunistic Pathogens by
1166 Comparing Multiple Real-Time PCR Platforms for Potential Space Applications, in:
1167 43rd International Conference on Environmental Systems, International Conference on
1168 Environmental Systems (ICES). American Institute of Aeronautics and Astronautics,
1169 Reston, Virginia. doi:10.2514/6.2013-3314

1170 Own, C.S., Martinez, J., De Rego, T., Own, L.S., Weppelman, G., Thomas-Keprta, K.T.,
1171 Rahman, Z., Pettit, D.R., 2019. MOCHII portable spectroscopic electron microscope on
1172 ISS: progress toward flight, in: 50th Lunar and Planetary Science Conference. pp. 4–5.

1173 Park, J.W., Lee, Y.J., Meyer, A.S., Douterelo, I., Maeng, S.K., 2018. Bacterial growth
1174 through microfiltration membranes and NOM characteristics in an MF-RO integrated
1175 membrane system: Lab-scale and full-scale studies. *Water Res.* 144, 36–45.
1176 doi:10.1016/j.watres.2018.07.027

1177 Parra, M., Jung, J., Boone, T.D., Tran, L., Blaber, E.A., Brown, M., Chin, M., Chinn, T.,
1178 Cohen, J., Doeblner, R., Hoang, D., Hyde, E., Lera, M., Luzod, L.T., Mallinson, M.,
1179 Marcu, O., Mohamedaly, Y., Ricco, A.J., Rubins, K., Sgarlato, G.D., Talavera, R.O.,
1180 Tong, P., Uribe, E., Williams, J., Wu, D., Yousuf, R., Richey, C.S., Schonfeld, J.,

1181 Almeida, E.A.C., 2017. Microgravity validation of a novel system for RNA isolation
1182 and multiplex quantitative real time PCR analysis of gene expression on the
1183 International Space Station. *PLoS One* 12, e0183480. doi:10.1371/journal.pone.0183480
1184 Peabody, M.A., Van Rossum, T., Lo, R., Brinkman, F.S.L., 2015. Evaluation of shotgun
1185 metagenomics sequence classification methods using in silico and in vitro simulated
1186 communities. *BMC Bioinformatics* 16, 362. doi:10.1186/s12859-015-0788-5
1187 Perrin, E., Bacci, G., Garrelly, L., Canganella, F., Bianconi, G., Fani, R., Mengoni, A., 2018.
1188 Furnishing spaceship environment: evaluation of bacterial biofilms on different
1189 materials used inside International Space Station. *Res. Microbiol.* 169, 289–295.
1190 doi:10.1016/j.resmic.2018.04.001
1191 Petala, M., Tsiridis, V., Darakas, E., Kostoglou, M., 2020. Longevity Aspects of Potable
1192 Water Disinfected by Ionic Silver: Kinetic Experiments and Modeling. *Water* 12, 258.
1193 doi:10.3390/w12010258
1194 Phipps, W.S., Yin, Z., Bae, C., Sharpe, J.Z., Bishara, A.M., Nelson, E.S., Weaver, A.S.,
1195 Brown, D., McKay, T.L., Griffin, D., Chan, E.Y., 2014. Reduced-gravity Environment
1196 Hardware Demonstrations of a Prototype Miniaturized Flow Cytometer and Companion
1197 Microfluidic Mixing Technology. *J. Vis. Exp.* 51743. doi:10.3791/51743
1198 Pickett, M.T., Roberson, L.B., Calabria, J.L., Bullard, T.J., Turner, G., Yeh, D.H., 2020.
1199 Regenerative water purification for space applications: Needs, challenges, and
1200 technologies towards “closing the loop.” *Life Sci. Sp. Res.* 24, 64–82.
1201 doi:10.1016/j.lssr.2019.10.002
1202 Pierson, D.L., Botkin, D.J., Bruce, R.J., Castro, V.A., Smith, M.J., Oubre, C.M., Ott, C.M.,
1203 2013. Microbial monitoring of the international space station, in: Moldenhauer, J. (Ed.),
1204 Environmental Monitoring: A Comprehensive Handbook. DHI Publishing, River Grove,
1205 pp. 1–27.

1206 Pittman, R.B., Harper, L.D., Newfield, M.E., Rasky, D.J., 2016. Lunar Station: The Next
1207 Logical Step in Space Development. *New Sp.* 4, 7–14. doi:10.1089/space.2015.0031

1208 Pomati, F., Jokela, J., Simona, M., Veronesi, M., Ibelings, B.W., 2011. An automated
1209 platform for phytoplankton ecology and aquatic ecosystem monitoring. *Environ. Sci.*
1210 *Technol.* doi:10.1021/es201934n

1211 Prest, E.I., Hammes, F., Kotzsch, S., van Loosdrecht, M.C.M., Vrouwenvelder, J.S., 2013.
1212 Monitoring microbiological changes in drinking water systems using a fast and
1213 reproducible flow cytometric method. *Water Res.* 47, 7131–7142.
1214 doi:10.1016/j.watres.2013.07.051

1215 Props, R., Kerckhof, F.-M., Rubbens, P., De Vrieze, J., Hernandez Sanabria, E., Waegeman,
1216 W., Monsieurs, P., Hammes, F., Boon, N., 2017. Absolute quantification of microbial
1217 taxon abundances. *ISME J.*

1218 Props, R., Monsieurs, P., Mysara, M., Clement, L., Boon, N., 2016. Measuring the
1219 biodiversity of microbial communities by flow cytometry. *Methods Ecol. Evol.* 7, 1376–
1220 1385. doi:10.1111/2041-210X.12607

1221 Radstrom, P., Lofstrom, C., Lovenklev, M., Knutsson, R., Wolffs, P., 2008. Strategies for
1222 Overcoming PCR Inhibition. *Cold Spring Harb. Protoc.* 2008, pdb.top20-pdb.top20.
1223 doi:10.1101/pdb.top20

1224 Ramírez-Castillo, F., Loera-Muro, A., Jacques, M., Garneau, P., Avelar-González, F., Harel,
1225 J., Guerrero-Barrera, A., 2015. Waterborne Pathogens: Detection Methods and
1226 Challenges. *Pathogens* 4, 307–334. doi:10.3390/pathogens4020307

1227 Rettberg, P., Antunes, A., Brucato, J., Cabezas, P., Collins, G., Haddaji, A., Kminek, G.,
1228 Leuko, S., McKenna-Lawlor, S., Moissl-Eichinger, C., Fellous, J.-L., Olsson-Francis,
1229 K., Pearce, D., Rabbow, E., Royle, S., Saunders, M., Sephton, M., Spry, A., Walter, N.,
1230 Wimmer Schweingruber, R., Treuet, J.-C., 2019. Biological Contamination Prevention

1231 for Outer Solar System Moons of Astrobiological Interest: What Do We Need to Know?
1232 *Astrobiology* 19, 951–974. doi:10.1089/ast.2018.1996

1233 Ricchi, M., Bertasio, C., Boniotti, M.B., Vicari, N., Russo, S., Tilola, M., Bellotti, M.A.,
1234 Bertasi, B., 2017. Comparison among the quantification of bacterial pathogens by qPCR,
1235 dPCR, and cultural methods. *Front. Microbiol.* doi:10.3389/fmicb.2017.01174

1236 Rizzardi, L.F., Kunz, H., Rubins, K., Chouker, A., Quiriarte, H., Sams, C., Crucian, B.E.,
1237 Feinberg, A.P., 2016. Evaluation of techniques for performing cellular isolation and
1238 preservation during microgravity conditions. *npj Microgravity* 2, 16025.
1239 doi:10.1038/npjmgrav.2016.25

1240 Robinson, J.P., Roederer, M., 2015. Flow cytometry strikes gold. *Science* (80-.). 350, 739–
1241 740. doi:10.1126/science.aad6770

1242 Roda, A., Mirasoli, M., Guardigli, M., Zangheri, M., Caliceti, C., Calabria, D., Simoni, P.,
1243 2018. Advanced biosensors for monitoring astronauts' health during long-duration space
1244 missions. *Biosens. Bioelectron.* 111, 18–26. doi:10.1016/j.bios.2018.03.062

1245 Rodriguez, N.M., Wong, W.S., Liu, L., Dewar, R., Klapperich, C.M., 2016. A fully
1246 integrated paperfluidic molecular diagnostic chip for the extraction, amplification, and
1247 detection of nucleic acids from clinical samples. *Lab Chip* 16, 753–763.
1248 doi:10.1039/C5LC01392E

1249 Roman, M.C., Weir, N.E., Wilson, M.E., Pyle, B.H., 2006. Microbial Characterization of
1250 Internal Active Thermal Control System (IATCS) Hardware Surfaces after Five Years
1251 of Operation in the International Space Station. *SAE Trans.* 115, 396–402.

1252 Ronca, A.E., Moyer, E.L., Talyansky, Y., Lowe, M., Padmanabhan, S., Choi, S., Gong, C.,
1253 Cadena, S.M., Stodieck, L., Globus, R.K., 2019. Behavior of mice aboard the
1254 International Space Station. *Sci. Rep.* 9, 4717. doi:10.1038/s41598-019-40789-y

1255 Rubbens, P., Schmidt, M.L., Props, R., Biddanda, B.A., Boon, N., Waegeman, W., Deneff,

1256 V.J., 2019. Randomized Lasso Links Microbial Taxa with Aquatic Functional Groups
1257 Inferred from Flow Cytometry. *mSystems* 4. doi:10.1128/mSystems.00093-19

1258 Safford, H.R., Bischel, H.N., 2019. Flow cytometry applications in water treatment,
1259 distribution, and reuse: A review. *Water Res.* 151, 110–133.
1260 doi:10.1016/j.watres.2018.12.016

1261 Salter, S.J., Cox, M.J., Turek, E.M., Calus, S.T., Cookson, W.O., Moffatt, M.F., Turner, P.,
1262 Parkhill, J., Loman, N.J., Walker, A.W., 2014. Reagent and laboratory contamination
1263 can critically impact sequence-based microbiome analyses. *BMC Biol.* 12, 87.
1264 doi:10.1186/s12915-014-0087-z

1265 Samhan, F.A., Stedtfeld, T.M., Waseem, H., Williams, M.R., Stedtfeld, R.D., Hashsham,
1266 S.A., 2017. On-filter direct amplification of *Legionella pneumophila* for rapid
1267 assessment of its abundance and viability. *Water Res.* 121, 162–170.
1268 doi:10.1016/j.watres.2017.05.028

1269 Segata, N., Waldron, L., Ballarini, A., Narasimhan, V., Jousson, O., Huttenhower, C., 2012.
1270 Metagenomic microbial community profiling using unique clade-specific marker genes.
1271 *Nat. Methods.* doi:10.1038/nmeth.2066

1272 Shapiro, H.M., 2005. Using Flow Cytometry. *Pract. Flow Cytom.* 736.
1273 doi:10.1002/0471722731.fmatter

1274 Siebel, E., Wang, Y., Egli, T., Hammes, F., 2008. Correlations between total cell
1275 concentration, total adenosine tri-phosphate concentration and heterotrophic plate counts
1276 during microbial monitoring of drinking water. *Drink. Water Eng. Sci. Discuss.* 1, 71–
1277 86. doi:10.5194/dwesd-1-71-2008

1278 Sobisch, L.-Y., Rogowski, K.M., Fuchs, J., Schmieder, W., Vaishampayan, A., Oles, P.,
1279 Novikova, N., Grohmann, E., 2019. Biofilm Forming Antibiotic Resistant Gram-
1280 Positive Pathogens Isolated From Surfaces on the International Space Station. *Front.*

1281 Microbiol. 10. doi:10.3389/fmicb.2019.00543

1282 Stevenson, A., Burkhardt, J., Cockell, C.S., Cray, J.A., Dijksterhuis, J., Fox-Powell, M., Kee,
1283 T.P., Kminek, G., McGenity, T.J., Timmis, K.N., Timson, D.J., Voytek, M.A., Westall,
1284 F., Yakimov, M.M., Hallsworth, J.E., 2015. Multiplication of microbes below 0.690
1285 water activity: implications for terrestrial and extraterrestrial life. *Environ. Microbiol.*
1286 17, 257–277. doi:10.1111/1462-2920.12598

1287 Straub, J., 2015. In search of technology readiness level (TRL) 10. *Aerosp. Sci. Technol.* 46,
1288 312–320. doi:10.1016/j.ast.2015.07.007

1289 Tan, B.F., Ng, C., Nshimiyimana, J.P., Loh, L.L., Gin, K.Y.H., Thompson, J.R., 2015. Next-
1290 generation sequencing (NGS) for assessment of microbial water quality: Current
1291 progress, challenges, and future opportunities. *Front. Microbiol.*
1292 doi:10.3389/fmicb.2015.01027

1293 Tan, S.C., Yiap, B.C., 2009. DNA, RNA, and Protein Extraction: The Past and The Present.
1294 *J. Biomed. Biotechnol.* 2009, 1–10. doi:10.1155/2009/574398

1295 Thyssen, M., Tarran, G.A., Zubkov, M. V., Holland, R.J., Gregori, G., Burkill, P.H., Denis,
1296 M., 2007. The emergence of automated high-frequency flow cytometry: revealing
1297 temporal and spatial phytoplankton variability. *J. Plankton Res.* 30, 333–343.
1298 doi:10.1093/plankt/fbn005

1299 Tremblay, J., Singh, K., Fern, A., Kirton, E.S., He, S., Woyke, T., Lee, J., Chen, F., Dangel,
1300 J.L., Tringe, S.G., 2015. Primer and platform effects on 16S rRNA tag sequencing.
1301 *Front. Microbiol.* 6. doi:10.3389/fmicb.2015.00771

1302 van der Wielen, P., van der Kooij, D., 2010. Effect of water composition , distance and
1303 season on the adenosine triphosphate concentration in unchlorinated drinking water in
1304 the Netherlands. *Water Res.* 44, 4860–4867. doi:10.1016/j.watres.2010.07.016

1305 Van Houdt, R., Leys, N., 2012. Monitoring the Microbial Burden in Manned Space Stations,

1306 in: Chouker, A. (Ed.), *Stress Challenges and Immunity in Space*. Springer Berlin
1307 Heidelberg, Berlin, Heidelberg, pp. 299–308. doi:10.1007/978-3-642-22272-6_22

1308 Van Houdt, R., Mijndonckx, K., Leys, N., 2012. Microbial contamination monitoring and
1309 control during human space missions. *Planet. Space Sci.* 60, 115–120.
1310 doi:10.1016/j.pss.2011.09.001

1311 Van Nevel, S., Koetzsch, S., Proctor, C.R., Besmer, M.D., Prest, E.I., Vrouwenvelder, J.S.,
1312 Knezev, A., Boon, N., Hammes, F., 2017. Flow cytometric bacterial cell counts
1313 challenge conventional heterotrophic plate counts for routine microbiological drinking
1314 water monitoring. *Water Res.* 113, 191–206.

1315 Vang, Ó.K., Corfitzen, C.B., Smith, C., Albrechtsen, H.-J., 2014. Evaluation of ATP
1316 measurements to detect microbial ingress by wastewater and surface water in drinking
1317 water. *Water Res.* 64, 309–320. doi:https://doi.org/10.1016/j.watres.2014.07.015

1318 Velusamy, V., Arshak, K., Korostynska, O., Oliwa, K., Adley, C., 2010. An overview of
1319 foodborne pathogen detection: In the perspective of biosensors. *Biotechnol. Adv.* 28,
1320 232–254. doi:10.1016/j.biotechadv.2009.12.004

1321 Venkateswaran, K., Hattori, N., La Duc, M.T., Kern, R., 2003. ATP as a biomarker of viable
1322 microorganisms in clean-room facilities. *J. Microbiol. Methods.* doi:10.1016/S0167-
1323 7012(02)00192-6

1324 Větrovský, T., Baldrian, P., 2013. The Variability of the 16S rRNA Gene in Bacterial
1325 Genomes and Its Consequences for Bacterial Community Analyses. *PLoS One* 8,
1326 e57923. doi:10.1371/journal.pone.0057923

1327 Vital, M., Stucki, D., Egli, T., Hammes, F., 2010. Evaluating the Growth Potential of
1328 Pathogenic Bacteria in Water. *Appl. Environ. Microbiol.* 76, 6477–6484.
1329 doi:10.1128/AEM.00794-10

1330 Weisse, T., Bergkemper, V., 2018. Rapid detection and quantification of the potentially toxic

- 1331 cyanobacterium *Planktothrix rubescens* by in-vivo fluorometry and flow cytometry.
1332 Water Res. 138, 234–240. doi:<https://doi.org/10.1016/j.watres.2018.03.052>
- 1333 Williams, M.R., Stedtfeld, R.D., Waseem, H., Stedtfeld, T., Upham, B., Khalife, W.,
1334 Etchebarne, B., Hughes, M., Tiedje, J.M., Hashsham, S.A., 2017. Implications of direct
1335 amplification for measuring antimicrobial resistance using point-of-care devices. Anal.
1336 Methods 9, 1229–1241. doi:[10.1039/C6AY03405E](https://doi.org/10.1039/C6AY03405E)
- 1337 Wolff, S., Palma, C., Marcelis, L., Kittang Jost, A.-I., van Delden, S., 2018. Testing New
1338 Concepts for Crop Cultivation in Space: Effects of Rooting Volume and Nitrogen
1339 Availability. Life 8, 45. doi:[10.3390/life8040045](https://doi.org/10.3390/life8040045)
- 1340 Wong, W.C., Oubre, C., Mehta, S.K., Ott, C.M., Pierson, D.L., 2017. Preventing Infectious
1341 Diseases in Spacecraft and Space Habitats, in: Hurst, C.J. (Ed.), Modeling the
1342 Transmission and Prevention of Infectious Disease. Springer International Publishing,
1343 Cham, Switzerland, pp. 3–17. doi:[10.1007/978-3-319-60616-3_1](https://doi.org/10.1007/978-3-319-60616-3_1)
- 1344 Yaginuma, H., Kawai, S., Tabata, K. V., Tomiyama, K., Kakizuka, A., Komatsuzaki, T.,
1345 Noji, H., Imamura, H., 2015. Diversity in ATP concentrations in a single bacterial cell
1346 population revealed by quantitative single-cell imaging. Sci. Rep. 4, 6522.
1347 doi:[10.1038/srep06522](https://doi.org/10.1038/srep06522)
- 1348 Yamaguchi, N., Roberts, M., Castro, S., Oubre, C., Makimura, K., Leys, N., Grohmann, E.,
1349 Sugita, T., Ichijo, T., Nasu, M., 2014. Microbial Monitoring of Crewed Habitats in
1350 Space—Current Status and Future Perspectives. Microbes Environ. 29, 250–260.
1351 doi:[10.1264/jsme2.ME14031](https://doi.org/10.1264/jsme2.ME14031)
- 1352 Yang, J., Thornhill, S.G., Barrila, J., Nickerson, C.A., Ott, C.M., McLean, R.J.C., 2018.
1353 Microbiology of the Built Environment in Spacecraft Used for Human Flight, in:
1354 Methods in Microbiology. pp. 3–26. doi:[10.1016/bs.mim.2018.07.002](https://doi.org/10.1016/bs.mim.2018.07.002)
- 1355 Yang, L., Wu, L., Zhu, S., Long, Y., Hang, W., Yan, X., 2010. Rapid, Absolute, and

1356 Simultaneous Quantification of Specific Pathogenic Strain and Total Bacterial Cells
1357 Using an Ultrasensitive Dual-Color Flow Cytometer. *Anal. Chem.* 82, 1109–1116.
1358 doi:10.1021/ac902524a

1359 Zea, L., Nisar, Z., Rubin, P., Cortesão, M., Luo, J., McBride, S.A., Moeller, R., Klaus, D.,
1360 Müller, D., Varanasi, K.K., Muecklich, F., Stodieck, L., 2018. Design of a spaceflight
1361 biofilm experiment. *Acta Astronaut.* 148, 294–300. doi:10.1016/j.actaastro.2018.04.039

1362 Zhang, B., Bai, P., Zhao, X., Yu, Y., Zhang, X., Li, D., Liu, C., 2019. Increased growth rate
1363 and amikacin resistance of *Salmonella enteritidis* after one-month spaceflight on China's
1364 Shenzhou-11 spacecraft. *Microbiol. Open* 8, e833. doi:10.1002/mbo3.833

1365 Zhang, K., Pan, R., Zhang, T., Xu, J., Zhou, X., Yang, Y., 2019. A novel method: using an
1366 adenosine triphosphate (ATP) luminescence-based assay to rapidly assess the biological
1367 stability of drinking water. *Appl. Microbiol. Biotechnol.* doi:10.1007/s00253-019-
1368 09774-3

1369 Zhao, Y., Chen, F., Li, Q., Wang, L., Fan, C., 2015. Isothermal Amplification of Nucleic
1370 Acids. *Chem. Rev.* 115, 12491–12545. doi:10.1021/acs.chemrev.5b00428

1371 Zou, Y., Mason, M.G., Wang, Y., Wee, E., Turni, C., Blackall, P.J., Trau, M., Botella, J.R.,
1372 2017. Nucleic acid purification from plants, animals and microbes in under 30 seconds.
1373 *PLOS Biol.* 15, e2003916. doi:10.1371/journal.pbio.2003916
1374