

AperTO - Archivio Istituzionale Open Access dell'Università di Torino

Quantitative determination of some volatile suspected allergens in cosmetic creams spread on skin by direct contact sorptive tape extraction-gas chromatography-mass spectrometry

This is the author's manuscript

Original Citation:

Availability:

This version is available <http://hdl.handle.net/2318/72426> since

Published version:

DOI:10.1016/j.chroma.2009.12.052

Terms of use:

Open Access

Anyone can freely access the full text of works made available as "Open Access". Works made available under a Creative Commons license can be used according to the terms and conditions of said license. Use of all other works requires consent of the right holder (author or publisher) if not exempted from copyright protection by the applicable law.

(Article begins on next page)



UNIVERSITÀ DEGLI STUDI DI TORINO

This Accepted Author Manuscript (AAM) is copyrighted and published by Elsevier. It is posted here by agreement between Elsevier and the University of Turin. Changes resulting from the publishing process - such as editing, corrections, structural formatting, and other quality control mechanisms - may not be reflected in this version of the text. The definitive version of the text was subsequently published in [*Journal of Chromatography A*, Volume: 1217, Issue 16, Pages: 2599-2605, date: APR 16 2010, DOI: <http://dx.doi.org/10.1016/j.chroma.2009.12.052>].

You may download, copy and otherwise use the AAM for non-commercial purposes provided that your license is limited by the following restrictions:

- (1) You may use this AAM for non-commercial purposes only under the terms of the CC-BY-NC-ND license.
- (2) The integrity of the work and identification of the author, copyright owner, and publisher must be preserved in any copy.
- (3) You must attribute this AAM in the following format: Creative Commons BY-NC-ND license (<http://creativecommons.org/licenses/by-nc-nd/4.0/deed.en>), <http://dx.doi.org/10.1016/j.chroma.2009.12.052>

Special issue on Extraction Techniques

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16

Quantitative determination of some volatile suspected allergens in cosmetic creams spread on skin by direct contact Sorptive Tape Extraction - Gas Chromatography - Mass Spectrometry

B. Sgorbini, M.R. Ruosi, C. Cordero, E. Liberto, P. Rubiolo, C. Bicchi

Dipartimento di Scienza e Tecnologia del Farmaco, Università degli Studi di Torino, Via P. Giuria 9, I-10125 Torino, Italy

Address for correspondence: Prof. Dr. Carlo Bicchi,
Dipartimento di Scienza e Tecnologia del Farmaco, Università di Torino,
Via Pietro Giuria 9, I-10125 Torino, Italy;
Tel. +39 011 670 7661 - 2; Fax: +39 670 7687; e-mail: carlo.bicchi@unito.it

17 **Abstract:** This study describes a method based on direct contact sorptive tape extraction followed
18 by on-line thermal desorption gas chromatography-mass spectrometry (DC-STE-GC-MS) to detect
19 and quantify a group of suspected volatile allergens on the European Union (E.U.) list and a related
20 compound on the skin (the stratum corneum) of volunteers treated with a cream of known
21 composition fortified with the reference allergens. The following compounds were tested:
22 citronellol, Z-citral (neral), geraniol, cinnamaldehyde, anisyl alcohol, cinnamyl alcohol, eugenol,
23 methyleugenol, coumarin, isoeugenol, α -isomethylionone, 2-(4-tert-butylbenzyl)propionaldehyde
24 (lilial), α -amylcinnamaldehyde, α -hexylcinnamaldehyde.

25 Sorptive Tape Extraction (STE) is a sorption-based sampling technique in which a flexible
26 polydimethylsiloxane (PDMS) tape is used to recover analytes by direct contact with the surface of
27 a solid matrix or from the headspace in equilibrium with it.

28 The reliability of the method was confirmed by: i) allergen recoveries varying from 52.3% for lilial
29 to 95.7% for neral, ii) linearity in the range 10-150 ppm, with regression coefficient R^2 always
30 above 0.97, iii) repeatability of each analyte, RSD% never exceeding 10%, iv) intermediate
31 precision, always below 15%, and v) LOD and LOQ in the ppb range, therefore fully compatible
32 with E.U. prescriptions (ppm). Other parameters such as substantivity analyte, approximate
33 permeation through skin and influence of different nature of stratum corneum on recovery were also
34 investigated. The method was also successfully applied to five commercially-available creams
35 declared to contain some of the allergens in question spread on the skin of the same volunteers.

36

37 **Keywords:** Direct contact sorptive tape extraction (DC-STE); PDMS tape; GC-MS; cosmetic
38 cream; volatile suspected allergen; skin; quantitative analysis.

39

40 ***1. Introduction***

41 The ever-increasing importance of volatiles as markers to characterize liquid or solid matrices has
42 strongly stimulated the development of highly effective sample preparation techniques, mainly for
43 vapor phase sampling. Several solventless techniques suitable for application to both liquid and
44 vapor phases have successfully been developed, after the introduction of the first and most popular
45 method, i.e. Solid Phase Microextraction (SPME) [1,2]. The newer techniques aim to offer better
46 performance than SPME and extend the fields of application; they include in-tube sorptive
47 extraction (INCAT, SPDE), sorptive extraction (SBSE, HSSE), solid-phase aroma concentrate
48 extraction (SPACE), large surface area sampling (MESI, MME, STE) and liquid phase
49 microextraction (LPME, HS-LPME). Their use in headspace sampling was recently reviewed by
50 Bicchi et al. [3]. Most techniques are based on the high concentration capacity approach, i.e.
51 techniques where the analytes are accumulated into a polymer by sorption or adsorption and

52 recovered by liquid or thermal desorption on-line or off-line to gas chromatography (GC), as such
53 or combined with MS (GC-MS).

54 In 2006 Sandra et al. introduced sorptive tape extraction (STE) [4], a technique whereby the
55 analytes are accumulated by sorption on a thin flexible PDMS tape, recovered by either thermal or
56 solvent desorption and analysed on-line by GC or GC-MS. They applied STE to study the effect of
57 a cosmetic treatment on the composition of human skin sebum (taken as marker) through *in vivo*
58 sampling by direct contact of the PDMS tape with the skin surface. More recently, Bicchi et al. [5]
59 successfully applied PDMS tapes to static headspace (HS-STE) and direct-contact (DC-STE)
60 sampling at the surface of solid matrices, such as the leaves of aromatic plants and fruits, and in the
61 fragrance field. The main advantages of PDMS tapes are high analyte recovery, due to their large
62 surface, and especially their specific ability to sample analytes by direct contact from the surface of
63 a solid matrix. The influence of surface on recovery was already discussed by Bruheim et al. [6]
64 who found that, with a thin sheet of a PDMS membrane, better recoveries were obtained in shorter
65 times and with higher sensitivity than with a thick-film PDMS-coated SPME fibre, in sampling
66 PAHs-spiked water. This increased performance for both vapour phase and in-solution sampling
67 was shown to be due to the larger ratio between surface area and extraction phase volume.

68 Standards of quality and safety for cosmetic and food products are becoming increasingly severe.
69 One example is the list of 26 compounds suspected of being possible causes of contact-allergy
70 reactions in fragrance-sensitive consumers, included in the latest E.U. legislation on cosmetics [7].
71 The amount of these substances must be declared on the label if it exceeds the limit of 0.001% for
72 “leave-on” and 0.01% for “rinse-off” cosmetic products. Several methods for the determination of
73 suspected allergens in fragrances and other cosmetic products have been reported. [8-11]

74 Another equally important aspect concerns monitoring these compounds after application of a
75 cosmetic formulation containing them, in particular detection and quantitation on the skin surface
76 after cosmetic treatment, and studying skin permeation and persistence, the latter more correctly
77 known as “substantivity” of the application [12].

78 This study aimed to detect and quantify thirteen suspected volatile allergens and a related
79 compound on the skin surface (i.e. the stratum corneum) after treatment with a reference cream of
80 known composition fortified with them. This was achieved by treating volunteers with cream
81 fortified with known amounts of a standard mixture of the compounds investigated, and with a
82 number of commercially-available creams (five) whose labels declared they contained them, and
83 then detecting and quantifying them on the skin surface by direct contact STE, followed by on-line
84 recovery by thermal desorption and GC-MS analysis (DC-STE-GC-MS).

85

86 ***2. Experimental***

87 2.1. Chemicals, reagents and matrices

88 Pure standards of citronellol (1), Z-citral (neral) (2), geraniol (3), cinnamaldehyde (4), anisyl
89 alcohol (5), cinnamyl alcohol (6), eugenol (7), methyleugenol (8), coumarin (9), isoeugenol (10), α -
90 isomethylionone (11), 2-(4-tert-butylbenzyl)propionaldehyde (lilial) (12), α -amylcinnamaldehyde
91 (13), α -hexylcinnamaldehyde (14) and undecane, used as internal standard (IS), were from the
92 laboratory collection of standards. Methyleugenol was included on the list to show that the method
93 can be extended to the quantitation of other compounds used in the cosmetic field. Table 1 lists the
94 analytes investigated, their CAS numbers and Log $K_{O/W}$. A standard mixture of 50 mg of each of
95 the fourteen compounds under investigation (SA mixture) was prepared and stored at -20°C until
96 use.

97 PDMS tapes (length: 15 mm, width: 4 mm, thickness: 0.5 mm; area: 0.6 cm²) were kindly supplied
98 by Prof. Dr. Pat Sandra (Research Institute for Chromatography – Kortrijk (Belgium)).

99 A cream consisting of Phytocream® (SEPPIC, France) (3%), octyl octanoate (14%), glycerol (5%)
100 and water (78%) was supplied by the Laboratory of Cosmetic Chemistry, Dipartimento di Scienza e
101 Tecnologia del Farmaco, University of Turin (Italy) and taken as reference (“cream” for short). The
102 cream was fortified with an amount of SA mixture suitable to achieve a final concentration of each
103 investigated allergen of around 200 ppm (for short “mother cream”). Table 1 reports the
104 concentrations in ppm of the analytes in the mother cream; it was then diluted with suitable amounts
105 of unfortified cream to achieve the concentration required for each experiment.

106 Two volunteers (volunteer 1 and volunteer 2) underwent these experiments. They gave their
107 informed consent after having been informed in detail about all risks involved with the study and on
108 how to proceed in case of adverse reaction. All procedures were performed in compliance with
109 relevant laws and institutional guidelines.

110 Five commercially-available creams, whose labels declare compositions similar to that of the
111 reference cream and indicates them to contain the suspected allergens investigated (for short
112 “commercial cream”), were also analyzed.

113

114 2.2. DC-STE skin surface sampling

115 A weighed amount (70 mg) of both the cream spiked with a known concentration of the
116 investigated allergens and a related compound obtained by a suitable dilution of the mother cream
117 and the commercial creams was spread uniformly on a precisely defined area of the back of one
118 hand of one volunteer; a surface large enough to afford at least six non-overlapping DC-STE
119 samplings was circumscribed (32 cm²). The PDMS tape was rested on the treated surface of the
120 hand for 30 minutes at the skin temperature. After sampling, PDMS tapes were removed from the
121 hand, inserted into a glass tube and then introduced into a thermodesorber (TDU, Gerstel, Mülheim

122 a/d Ruhr, Germany) from where the analytes were recovered and analyzed by GC-MS (see
123 paragraph 2.3.). This procedure was used to evaluate the following parameters for each investigated
124 analyte: calibration curve and linearity, repeatability and intermediate precision, limits of detection
125 (LOD) and quantitation (LOQ), recovery, substantivity, cream permeation, influence of nature of
126 stratum corneum of the two volunteers on recovery, and to analyze five commercial creams.

127 Undecane was used as internal standard: it was homogeneously sorbed into all PDMS tapes before
128 each experiment by suspending them in 4 mL of a standard solution of undecane in water (4 µg/mL)
129 and stirring them for 30 minutes, following the method proposed by Pawliszyn for SPME [13].
130

131 2.2.1. Calibration curves, linearity and quantitation

132 A calibration curve was constructed for each investigated compound, by spreading a weighed
133 amount (70 mg) of cream suitably diluted from the mother cream to obtain concentrations of about
134 10, 25, 50, 100 and 150 ppm of each analyte on the circumscribed surface (about 32 cm²) of the
135 back of one hand of volunteer 1, and then submitted to sampling with a PDMS tape (DC-STE). The
136 sampled analytes were thermally recovered from the tape and analyzed on-line by GC-MS under the
137 conditions reported in paragraphs 2.2 and 2.3.

138 The investigated analytes were quantitated by GC-MS operating in single ion monitoring
139 acquisition mode (SIM) by determining the areas of at least three selected ions (one target ion and
140 two qualifiers) for each analyte, both to confirm its identity on the basis of the quality values
141 referred to target ion area ratios of a reference standard and to quantify it. Table 2 reports m/z target
142 and qualifier ions used for SIM acquisition of the fourteen compounds investigated. The calibration
143 curves for each analyte investigated were calculated on the basis of the area of its target ion
144 (normalised *versus* the undecane IS) *versus* the corresponding concentration.
145

146 2.2.2. Repeatability, intermediate precision

147 Weighed aliquots (70mg) of the cream spiked with 25, 50, and 100 ppm of each investigated
148 compound were spread uniformly on the selected surface (32 cm²) of the back of one hand of
149 volunteer 1, and sampled with a PDMS tape (DC-STE). The sampled analytes were recovered from
150 the tape thermally and analyzed by GC-MS under the conditions reported in paragraphs 2.2 and 2.3.
151 Each experiment was repeated six consecutive times to evaluate repeatability. Intermediate
152 precision was determined on the 50 ppm spiked cream, analyzed every four weeks over a period of
153 three months.
154

155 2.2.3. LOD and LOQ determination

156 The LOD and LOQ of each analyte was determined following Eurachem guidelines [14]. Ten blank
157 experiments were carried out on the unspiked cream with the method described above. The LOD of
158 each analyte was calculated from the average “peak to peak” noise values sampled in its region of
159 elution in the chromatogram, with a coverage factor of 3. LOQ was experimentally determined by
160 analyzing samples spiked with decreasing concentration of each analyte. LOQ was the lowest
161 concentration to which the error for peak area determination (assignment) was $\leq 20\%$.

162

163 *2.2.4. Analyte recovery, substantivity and approximate skin-permeation and influence of nature of* 164 *volunteers' stratum corneum on recovery*

165 Analyte recovery was determined by spreading a weighed amount (70 mg) of the cream spiked with
166 50 and 100 ppm of each analyte, obtained by suitable dilution of the mother cream, uniformly on
167 the selected surface (32 cm²) of the back of one hand of volunteer 1, then submitted to sampling
168 with a PDMS tape (DC-STE). The sampled analytes were thermally recovered from the tape and
169 analyzed by GC-MS under the conditions reported in paragraphs 2.2 and 2.3. The recovery was
170 determined by the % ratios between the absolute amount of the analyte obtained by DC-STE-GC-
171 MS and that spiked in the cream.

172 The suspected allergens substantivity on the stratum corneum was measured by DC-STE sampling
173 after 0, 20, 40 and 60 minutes from spreading the cream (70 mg) spiked with 50 ppm of each
174 analyte in different positions of the surface of the back of the hand of volunteer 1 under the above
175 conditions.

176 A series of experiments were also carried out under the same conditions reported above but by
177 applying DC-STE sampling to an equivalent surface of a Pyrex glass plate spread with a known
178 amount of the 50 ppm spiked cream instead of the back of the hand of the volunteer 1. These
179 experiments were run to evaluate the allergen skin-permeation.

180 The influence of different stratum corneum on recovery was evaluated by DC-STE sampling of the
181 back of one hand of volunteers 1 and 2 treated with the same amount (70 mg) of the base cream
182 spiked with 50 ppm of the investigated analytes spread uniformly on the selected surface (32 cm²)
183 and then analyzed under the above conditions.

184

185 *2.2.5. Analysis of commercial creams*

186 Five commercial creams were analyzed under the same conditions adopted for the spiked cream.
187 The suspected allergens reported to be contained in the five commercial creams investigated are
188 listed in Table 6.

189

190 *2.3. Analysis conditions*

191 Analyte thermal desorption was carried out with a TDU unit from Gerstel (Gerstel, Mülheim a/d
192 Ruhr, Germany) driven by a MPS-2 multipurpose sampler (Gerstel, Mülheim a/d Ruhr, Germany)
193 installed on an Agilent 6890 GC unit coupled to an Agilent 5973N MSD (Agilent, Little Falls, DE,
194 USA) (Gerstel, Mülheim a/d Ruhr, Germany). For TDU the following parameters were used:
195 desorption program: from 30°C to 250°C (5 min) at 60°C/min; flow mode: splitless, transfer line:
196 300°C. A Gerstel CIS-4 PTV injector was used to cryogenically focus the analytes thermally
197 desorbed from the PDMS tapes. The PTV was cooled to -50°C using liquid CO₂; injection: PTV;
198 injection temperature: from -50°C to 250°C (5 min) at 12°C/s. The inlet was operated in the split
199 mode (split ratio 1:10).

200 Chromatographic conditions: helium was used as carrier gas at a flow rate of 1 mL/min.

201 Column: FSOT Mega 5-MS (d_f 0.25 μm, i.d 0.25 mm, length 30 m) (Mega, Legnano (Milan),
202 Italy). Temperature program: from 0°C (1 min) to 80°C/min at 70°C (0 min), then to 180°C (0 min)
203 at 3°C/min, then to 250°C (5 min) at 15°C/min.

204 MSD conditions - MS operated in EI mode (70 eV), full scan with a mass range from 35 to 350 amu
205 and SIM acquisition (dwell time 40).

206

207 **3. Results and discussion**

208 Several parameters were investigated to evaluate the reliability of DC-STE-GC-MS for the purpose
209 of quantifying a group of suspected allergens and a related compound in a cream spread on the
210 stratum corneum, in particular: calibration curve and linearity, repeatability and intermediate
211 precision, limits of detection (LOD) and quantitation (LOQ), recovery, substantivity on the skin,
212 allergen skin-permeation, influence of nature of stratum corneum on recovery; in addition five
213 commercial creams were also analyzed.

214 Unless specified otherwise, all data are the mean of three repetitions after sampling for 30 minutes
215 with PDMS tapes of the back of one hand of a volunteer spread with the cream spiked with suitable
216 analyte concentrations, followed by thermal desorption of the recovered analytes from the tape and
217 on-line analysis by GC-MS. Figure 1a reports a TIC-GC-MS profile after DC-STE sampling of the
218 cream spiked with 50 ppm of each allergen.

219

220 *3.1. Calibration curves and quantitation*

221 Table 2 reports the equations of the concentration (ppm)/normalized areas calibration curves of the
222 investigated compounds and the corresponding regression coefficients R² after DC-STE-GC-MS
223 analysis. Target ions and qualifiers of each analyte were selected as reported by Chaintreau et al.
224 [15]. The areas of the target MS ions were used for quantitation. These results show that, in the
225 range of concentrations considered (i.e. 10-150 ppm), the linearity was very good with R² always

226 above 0.97; the only exception is cinnamaldehyde (4) whose R^2 is 0.9330. The unusual behavior of
227 cinnamaldehyde is probably due to the irregular peak shape at the lowest spiked quantities (namely
228 10 and 25 ppm), that interferes with its correct area integration.

229

230 3.2. Repeatability and intermediate precision

231 Table 3 reports repeatability (RSD%) calculated over six determinations of the DC-STE-GC-MS
232 analyses on the 25, 50, and 100 ppm spiked creams, the RSD% means, and the intermediate
233 precision determined over a period of three months by analyzing the 50 ppm spiked cream every
234 four weeks. RSD% values were determined on the analyte areas normalized vs. undecane (IS). The
235 results show that the average repeatability is very good, the average value for each compound never
236 exceeding 10%, with the exception of α -hexylcinnamaldehyde (14) (12.2%). The intermediate
237 precision was also satisfactory since it was always below 15%, ranging from 2.5% for α -
238 amylcinnamaldehyde (13) to 14.6% for isoeugenol (10).

239

240 3.3. Limits of detection (LOD) and quantitation (LOQ)

241 Table 2 reports the LOD and LOQ values calculated following Eurachem guidelines. The results
242 show that they are very low compared to legal limits, meaning that the method enables allergens
243 below the limits set by the E.U. legislation to be easily detected. The LOD ranged from 15 ppb for
244 cinnamaldehyde (4), anisyl alcohol (5) and methyleugenol (8) to 200 ppb for cinnamyl alcohol (6),
245 while the LOQ for the same compounds was 50 and 560 ppb, respectively.

246

247 3.4. Analyte recovery, substantivity and approximate skin permeation and influence of nature of 248 volunteer's stratum corneum on recovery

249 Table 4 reports the recoveries of investigated compounds after 30 minutes sampling calculated on
250 their amount determined by DC-STE-GC-MS vs. the amount spiking the cream. The concentrations
251 were calculated from the above calibration curves. The analyte recoveries were all rather high,
252 ranging from a minimum of 52.3% for α -amylcinnamaldehyde (13) and 58.4% for α -
253 hexylcinnamaldehyde (14) to a maximum of 95.7% for neral (2). The repeatability of recovery was
254 also very good, being around 10% for all analytes investigated. The difference in recoveries are due
255 to several co-occurring factors: i) analyte solubility in PDMS, which is directly proportional to the
256 octanol/water distribution constant $K_{O/W}$ [16], ii) analyte partition between the cream components
257 being it an emulsion of a hydrophobic phase in water, iii) analyte skin permeation, and to a lesser
258 extent iii) analyte volatility.

259 The analyte substantivity on the stratum corneum was also determined. In this case, DC-STE
260 sampling was carried out in different parts of the hand surface, spread with cream spiked with 50

261 ppm of the investigated compounds, at different times (0, 20, 40 and 60 min) after application.
262 Table 4 reports the area% reduction of each investigated analyte 20, 40, and 60 minutes after
263 application, measured by DC-STE-GC-MS analysis, taking values for time zero as 100%. As
264 expected, the results varied widely, being conditioned by the same factors mentioned above for
265 recovery, although in this case volatility assumes a bigger role as is evident from the % reductions
266 over time. After one hour, the most volatile compounds were almost completely absent from the
267 skin, while content of the less volatile, such as α -amylcinnamaldehyde (13) and α -
268 hexylcinnamaldehyde (14), remained almost constant. These experiments were also useful to define
269 the trend of analyte decay over time. All compounds decayed exponentially, with R^2 ranging from 1
270 for isoeugenol (10) to 0.8997 for neral (2). Figure 2 reports the diagrams for isoeugenol (10) and
271 cinnamyl alcohol (6).

272 These data may also be useful to obtain an indication of analyte evaporation and skin permeation.
273 Permeation through the stratum corneum was measured by running a set of experiments under
274 exactly the same operative conditions as for substantivity, but replacing the back of the hand of the
275 volunteer with a Pyrex glass plate. The approximate permeation percent was determined by
276 subtracting the absolute amount of each analyte found on the skin from that determined on the
277 Pyrex glass plate, and calculating its percentage *versus* the total amount recovered from the glass
278 plate. Table 5 reports the percentage of each analyte's approximate permeation through the stratum
279 corneum; these were found to be relatively low, never exceeding 20%.

280 The influence of the nature of the stratum corneum on analyte recovery was also preliminarily
281 evaluated. Volunteers 1 and 2 were treated with the same amount of cream spiked with 50 ppm of
282 each compound and their hands analyzed by DC-STE-GC-MS. The results, reported in Table 5, are
283 encouraging since the concentrations are different but quite similar with the two volunteers, and
284 also considering that, in these preliminary experiments, important parameters, such as the different
285 nature and condition of the stratum corneum and the difference in cream permeation between the
286 two volunteers, were not controlled. Further experiments are under way to evaluate the method's
287 applicability and the reliability of the results on a larger series of controlled subjects.

288

289 *3.5. Analysis of commercial creams*

290 Five commercial creams similar to the model cream, and reported to contain the investigated
291 allergens, were analyzed under the conditions reported for spiked cream, and quantified by means
292 of the calibration curves reported in the Table 2. Table 6 shows that the investigated commercial
293 creams contained the suspected allergens reported in the label: one of them (cream 4) in amount
294 close to the "leave-on" E.U. limits to be declared, the others in different and variable amounts.

295 Figure 1b reports the TIC-GC-MS profile after DC-STE sampling of commercial cream 1 and
296 figure 1c shows that of commercial cream 2.

297 The influence of the matrix on the results was also investigated by analyzing two of the commercial
298 creams (cream 3 and cream 5) spiked with 50 ppm of the SA mixture and analyzing them with the
299 DC-STE-GC-MS method described. The analytes' recoveries (not reported) were in line with those
300 in Table 4 for the spiked cream, thus excluding interference due to the matrix effect. On the other
301 hand, the same creams were also analyzed after a standard addition of 50 ppm of the allergens
302 identified in them. The results were very similar to those obtained with the calibration curves
303 showing the reliability of the method described.

304

305 *3.6. General considerations*

306 This study confirms the effectiveness and concentration capability of STE used for direct contact
307 sampling from the skin. Its application to the analysis of suspected allergens and related compounds
308 in creams applied to the skin is a highly reliable and sensitive method, offering high recoveries of
309 the analytes investigated together with good repeatability and sensitivity.

310 The main advantages of DC-STE, in particular for applications in this field and more in general in
311 biology, are that i) it comprises a one-step sampling procedure not requiring any further matrix or
312 sample manipulation, ii) it enables several simultaneous samplings to be run by applying the
313 required number of tapes onto the solid surface investigated, iii) it permits sampling(s) where the
314 biological phenomenon to be monitored takes place, and iv) all other steps of the method (thermal
315 desorption and GC-MS analysis) can be run automatically. On the other hand, it requires the
316 availability of a dedicated instrumentation for on-line thermal desorption and of a multipurpose
317 autosampler for automatic analysis.

318 In conclusion, DC-STE is an effective technique for sampling from solid biologically-active
319 surfaces. In particular the results reported show its efficacy in studying phenomena related to the
320 skin, where it can be effectively applied to determine directly or indirectly skin permeability to
321 drugs and cosmetics, to monitor both ingredients and their bioavailability, and skin markers to
322 evaluate their local effect .

323

324 **Acknowledgments**

325 This study was carried out within the project entitled: "Sviluppo di metodologie innovative per
326 l'analisi di prodotti agroalimentari" (FIRB Cod.: RBIP06SXMR_002) of the Ministero
327 dell'Istruzione, dell'Università e della Ricerca (MIUR) (Italy).

328

329 **References**

- 330 [1] C.L. Arthur, J. Pawliszyn, *Anal. Chem.* 62 (1990) 2145.
- 331 [2] Z. Zhang, J. Pawliszyn, *Anal. Chem.* 65 (1993) 1843.
- 332 [3] C. Bicchi, C. Cordero, E. Liberto, B. Sgorbini, P. Rubiolo, *J. Chromatogr. A* 1184 (2008) 2203.
- 333 [4] P. Sandra, S. Sisalli, A. Adao, M. Lebel, I. Le Fur, *LC-GC Europe* 19 (2006) 3311.
- 334 [5] C. Bicchi, C. Cordero, E. Liberto, P. Rubiolo, B. Sgorbini, P. Sandra, *J. Chromatogr. A* 1148
335 (2007) 137.
- 336 [6] I. Bruheim, X. Liu, J. Pawliszyn, *Anal. Chem.* 75 (2003) 1002.
- 337 [7] European Parliament Directive 2003/15/EC of the European Parliament and of the Council of 27
338 February 2003 amending Council Directive 76/768/EEC on the approximation of the laws of the
339 Member States relating to Cosmetic Products. *Off. J. Eur. Communities* 2003, L66.
- 340 [8] S.C. Rastogi, *J. High Resol. Chromatogr.* 18 (1995) 653.
- 341 [9] M. Niederer, R. Bollhalder, Ch. Hohl, *J. Chromatogr. A* 1132 (2006) 109.
- 342 [10] F. David, C. Devos, P. Sandra, *LC-GC Europe* 19 (2006).
- 343 [11] F. David, C. Devos, D. Joulain, A. Chaintreau, P. Sandra, *J. Sep. Sci.* 29 (2006) 1587.
- 344 [12] A. Chaintreau, F. Bégnaud, C. Debonneville, U. Keller, *Proceeding of the 40th International*
345 *Symposium on Essential Oil*, Ed. C. Bicchi and P. Rubiolo, 2009, p. 50.
- 346 [13] Y. Wang, J. O'Reilly, Y. Chen, J. Pawliszyn, *J. Chromatogr. A* 1072 (2005) 13.
- 347 [14] Eurachem Guide: Guide to quality in analytical chemistry. An aid to accreditation, 2002.
348 (<http://www.eurachem.org/guides/Citac%20Eurachem%20guide.pdf>).
- 349 [15] A. Chaintreau, D. Joulain, C. Marin, C. Schmidt, M. Vey, *J. Agric. Food Chem.* 51 (2003)
350 6398.
- 351 [16] E. Baltussen, C.A. Cramers, P. Sandra, *Anal. Bioanal. Chem.* 373 (2002) 3.

352
353

354 Caption to Tables

355

356 Table 1. List of the suspected allergens and a related compound investigated with their CAS
357 numbers, Log $K_{o/w}$ values and concentrations in the mother cream.

358

359 Table 2. List of the target ions (in bold) and qualifiers, calibration curves, regression coefficients
360 R^2 , LOD and LOQ values of the investigated compounds analyzed by DC-STE-GC-MS.

361

362 Table 3. Repeatability (RSD%) of the DC-STE-GC-MS method on cream spiked with different
363 amounts of the compounds investigated and intermediate precision.

364 Table 4. Average % recoveries and RDS% of the investigated allergens and a related compound and
365 their % area reduction after DC-STE samplings at different times after application of 50 ppm spiked
366 cream.

367

368 Table 5. Approximate permeation percentage of each compound and quantitative results after
369 application of 50 ppm spiked cream for the two volunteers.

370

371 Table 6. DC-STE-GC-MS quantitative determination of the declared allergens in the five
372 commercial creams investigated.

373

374 Caption to Figures

375


376 Figure 1. TIC-GC-MS profiles after DC-STE sampling of the cream spiked with 50 ppm of each
377 analyte (1a), and of commercial cream 1 (1b) and commercial cream 2 (1c). (For analysis
378 conditions and peak identification see text and tables)

379

380 Figure 2. Diagrams of the exponential decay over time of isoeugenol (10) and cinnamyl alcohol (6).

381

Figure 1

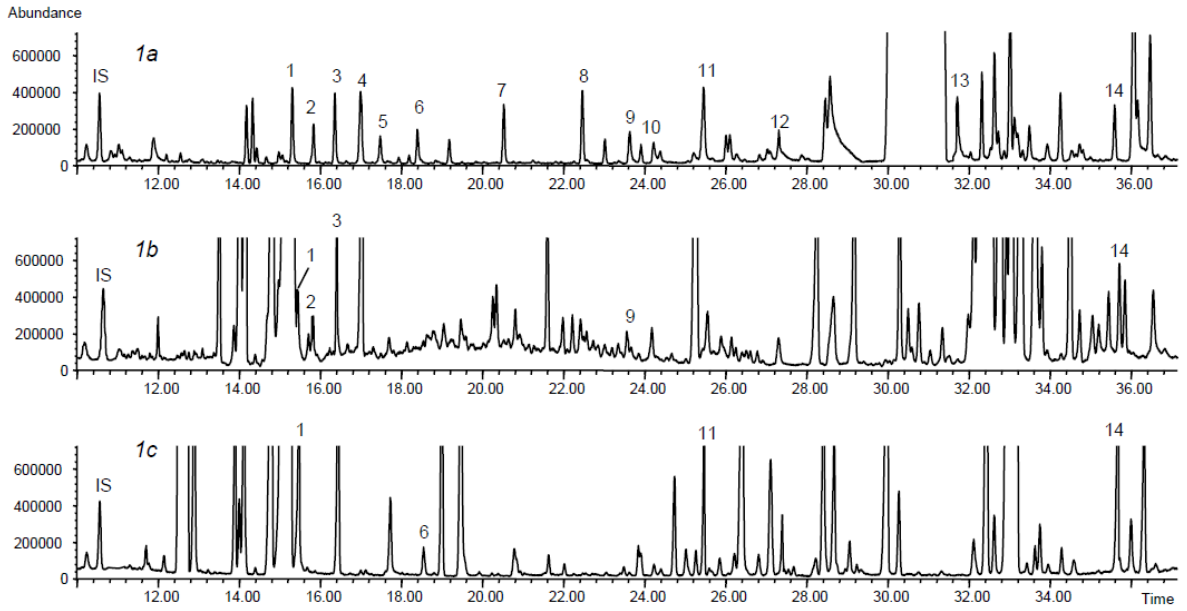


383

384

385

386

Figure

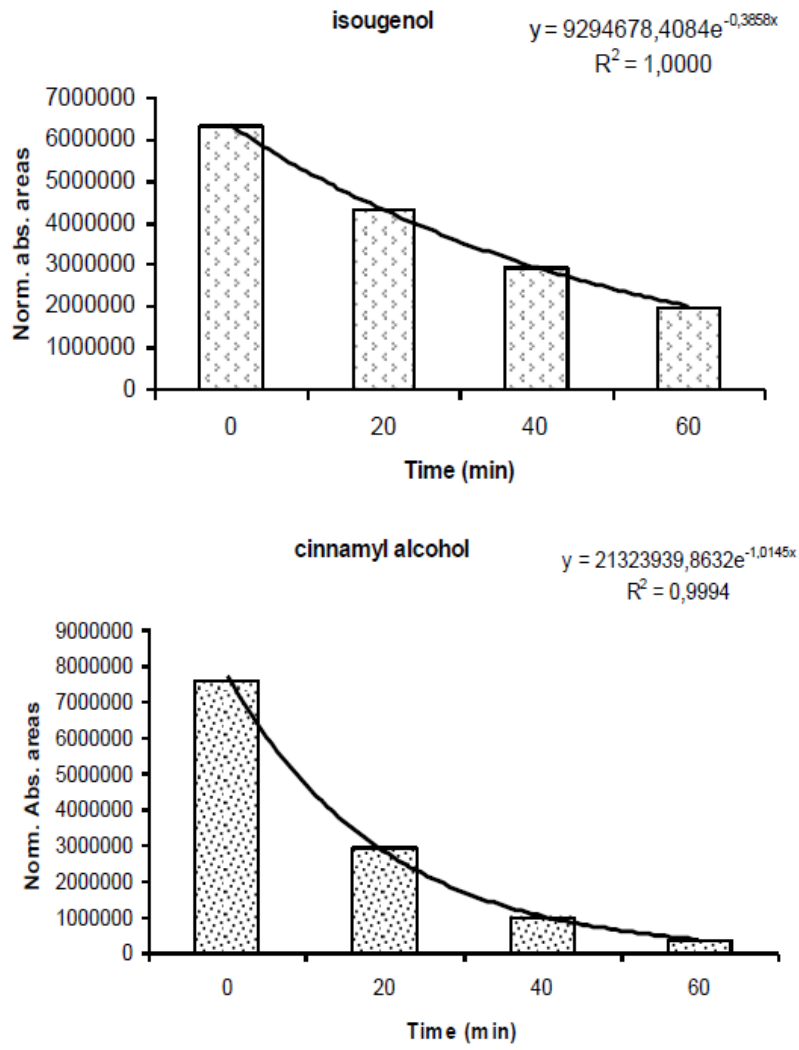

387

388

389

390 Table 1. List of the suspected allergens and a related compound investigated with their CAS
 391 numbers, Log $K_{o/w}$ values and concentrations in the mother cream.
 392
 393

#	Compound	CAS	Log $K_{o/w}$	Concentration in mother cream (ppm)
1	citronellol	106-22-9	3.56	183
2	Z-citral (neral)	106-26-3	3.45	227
3	geraniol	106-24-1	3.47	194
4	cinnamaldehyde	104-55-2	1.82	192
5	anisyl alcohol	105-13-5	1.16	190
6	cinnamyl alcohol	104-54-1	1.84	186
7	eugenol	97-53-0	2.73	186
8	methyleugenol ^a	93-15-2	3.03	187
9	coumarin	91-64-5	1.51	203
10	isoeugenol	97-54-1	2.65	194
11	α -isomethylionone	127-51-5	4.84	181
12	lilial	80-54-6	4.36	198
13	amylcinnamaldehyde	122-40-7	4.33	231
14	hexylcinnamaldehyde	101-86-0	4.82	173

417 ^a Compound not included in the E.U. list.
 418
 419
 420

421 Table 2. List of the target ions (in bold) and qualifiers, calibration curves, regression coefficients
 422 R², LOD and LOQ values of the investigated compounds analysed analyzed by DC-STE-GC-MS.
 423
 424

#	Compound	Ions	Calibration curve equation	R ²	LOD (ppb)	LOQ (ppb)
1	citronellol	69 , 95, 81	y=41227x-245189	0.9964	40	110
2	Z-citral (neral)	69 , 94, 109	y=26281x-92035	0.9899	140	400
3	geraniol	69 , 123, 93	y=76909x-427211	0.9940	50	130
4	cinnamaldehyde	131 , 132, 103	y=15144x+164547	0.9330	15	50
5	anisyl alcohol	138 , 137, 109	y=11676x+31631	0.9887	15	50
6	cinnamyl alcohol	92 , 134, 115	y=15277x-190695	0.9995	200	560
7	eugenol	164 , 103, 149	y=44491x-344722	0.9726	20	50
8	methyleugenol ^a	178 , 163, 147	y=43873x-205330	0.9921	15	50
9	coumarin	146 , 118, 89	y=45862x-234345	0.9958	35	100
10	isoeugenol	164 , 149, 131	y=27971x-134847	0.9996	190	500
11	α-isomethylionone	135 , 206, 150	y=82236x-447020	0.9945	70	200
12	lilial	189 , 204 147	y=34069x-247767	0.9999	50	130
13	amylcinnamaldehyde	202 , 201, 129	y=29270x-210605	0.9923	60	150
14	hexylcinnamaldehyde	216 , 215, 129	y=29208x-73216	0.9849	110	250

425 ^a Compound not included in the E.U. list.
 426
 427
 428

429 Table 3. Repeatability (RSD%) of the DC-STE-GC-MS method on cream spiked with different
 430 amounts of the compounds investigated and intermediate precision.
 431

#	Compound	Repeatability (RSD%)				Intermediate precision (RDS%)
		25 ppm	50 ppm	100 ppm	average	50 ppm
1	citronellol	5.7	4.4	2.4	3.4	9.0
2	Z-citral (neral)	4.8	4.4	2.8	3.3	6.5
3	geraniol	6.0	4.7	3.7	4.2	9.2
4	cinnamaldehyde	1.2	0.1	0.9	0.2	6.5
5	anisyl alcohol	6.6	5.6	4.2	5.0	9.8
6	cinnamyl alcohol	3.8	2.4	1.8	2.1	10.6
7	eugenol	8.4	7.2	7.3	7.2	12.1
8	methyleugenol ^a	7.9	8.1	7.2	7.2	8.2
9	coumarin	4.2	3.7	3.8	3.3	3.2
10	isoeugenol	8.6	7.8	6.9	7.1	14.6
11	α -isomethylionone	10.2	9.3	8.8	9.0	8.2
12	lilial	2.2	0.5	1.2	1.0	13.9
13	amylcinnamaldehyde	8.9	7.4	6.2	7.1	2.5
14	hexylcinnamaldehyde	15.4	13.4	9.4	12.2	14.2

432
 433 ^a Compound not included in the E.U. list.
 434

435 Table 4. Average % recoveries and RDS% of the investigated allergens and a related compound and
 436 their % area reduction after DC-STE samplings at different times after application of 50 ppm spiked
 437 cream.

#	Compound	Recovery %	Recovery repeatability (RSD%)	% Area reduction		
				after 20 min	after 40 min	after 60 min
1	citronellol	90.4	1.5	77.4	92.6	96.9
2	Z-citral (neral)	95.7	1.0	95.3	98.9	99.4
3	geraniol	87.7	6.6	75.8	91.8	96.8
4	cinnamaldehyde	94.8	1.0	87.4	94.3	97.8
5	anisyl alcohol	86.3	3.0	52.6	81.5	92.4
6	cinnamyl alcohol	70.6	2.5	61.5	87.1	95.1
7	eugenol	90.0	5.4	53.7	77.6	92.3
8	methyleugenol ^a	81.6	5.3	51.2	73.0	90.1
9	coumarin	78.7	7.7	58.1	82.0	93.4
10	isoeugenol	83.3	9.6	32.0	53.5	68.6
11	α -isomethylionone	66.8	10.1	40.3	59.1	73.9
12	lilial	74.0	6.5	15.4	19.1	35.8
13	amylcinnamaldehyde	52.3	6.2	23.4	23.6	27.8
14	hexylcinnamaldehyde	58.4	10.2	26.1	26.3	26.6

438

439 ^a Compound not included in the E.U. list.

440

441

442 Table 5. Approximate permeation percentage of each compounds and quantitative results after
 443 application of 50 ppm spiked cream for the two volunteers.
 444

#	Compound	Approx. % permeation (volunteer 1)	Influence of different stratum corneum		
			Cream concentration (ppm)	Volunteer 1 (ppm)	Volunteer 2 (ppm)
1	citronellol	12.7	46	43	43
2	Z-citral (neral)	15.6	57	52	58
3	geraniol	12.6	48	45	44
4	cinnamaldehyde	7.8	48	45	15
5	anisyl alcohol	16.5	48	43	30
6	cinnamyl alcohol	7.6	47	46	19
7	eugenol	19.6	47	40	40
8	methyleugenol ^a	14.5	47	43	36
9	coumarin	12.7	51	48	50
10	isoeugenol	8.0	48	48	40
11	α -isomethylionone	11.1	45	42	39
12	lilial	6.9	49	49	31
13	amylcinnamaldehyde	14.6	58	53	45
14	hexylcinnamaldehyde	16.1	43	39	31

445

446 ^a Compound not included in the E.U. list.

447

448 Table 6. DC-STE-GC-MS quantitative determination of the declared allergens in the five
449 commercial creams investigated.
450
451

#	Compound	Cream 1 (ppm)	Cream 2 (ppm)	Cream 3 (ppm)	Cream 4 (ppm)	Cream 5 (ppm)
1	citronellol	20	83	40	24	/
2	Z-citral (neral)	51	/	/	/	46
3	geraniol	90	/	36	16	/
6	cinnamyl alcohol	/	54	/	/	/
9	coumarin	12	/	/	/	28
11	α -isomethylionone	/	65	/	16	/
14	hexylcinnamaldehyde	75	121	/	10	/

452
453
454
455
456
457