

SHORT REPORT

Open Access

# Gene-targeted embryonic stem cells: real-time PCR assay for estimation of the number of neomycin selection cassettes

Cecilia Mancini<sup>1</sup>, Erika Messana<sup>1</sup>, Emilia Turco<sup>1,3</sup>, Alessandro Brussino<sup>1</sup> and Alfredo Brusco<sup>1,2\*</sup>

## Abstract

In the preparation of transgenic murine ES cells it is important to verify the construct has a single insertion, because an ectopic neomycin phosphotransferase positive selection cassette (*NEO*) may cause a position effect. During a recent work, where a knockin *SCA28* mouse was prepared, we developed two assays based on Real-Time PCR using both SYBR Green and specific minor groove binder (MGB) probes to evaluate the copies of *NEO* using the comparative delta-delta Ct method versus the *Rpp30* reference gene.

We compared the results from Southern blot, routinely used to quantify *NEO* copies, with the two Real-Time PCR assays. Twenty-two clones containing the single *NEO* copy showed values of  $0.98 \pm 0.24$  (mean  $\pm$  2 S.D.), and were clearly distinguishable from clones with two or more *NEO* copies.

This method was found to be useful, easy, sensitive and fast and could substitute for the widely used, but laborious Southern blot method.

Two methods are available for the introduction and modification of mouse genomic DNA sequences: (i) microinjection of one or more transgenes into the nucleus of a fertilized mouse oocyte, which usually leads to random incorporation into the genome as head-to-tail concatamers of 1-1000 units, or (ii) the use of constructs that undergo a site-specific recombination in embryonic stem cells (ES) in order to disrupt the function of a target gene (knockout) or to mutate a gene (knockin). Modified ES cells are then injected into the blastocyst [1]. In the latter case, the production of knockout or knockin ES cells is obtained through gene targeting by homologous recombination. In this work, ES cells were transfected by electroporation with a construct containing a specific genomic sequence harbouring the required mutation, along with the neomycin phosphotransferase positive selection cassette (*NEO*) for selection of positive recombinants, flanked by two homology sequences ("arms") driving the recombination [2,3]. Homologous recombination occurs in a small number of transfected cells, resulting in the introduction

of the mutation present in the targeting construct into the gene of interest. However, despite the presence of the two "arms", there may be a variable number of random integrations that may cause a position effect [4-6]. To identify the mutant ES cell clones to be microinjected, two Southern blots are usually performed: one to detect ES clones in which homologous recombination has occurred, and the other to verify the number of *NEO* cassettes. Usually between two and three hundred clones are analysed: useful clones are routinely just 1 - 2% of the total. This low percentage is mainly due to the event of the vector being inserted in ectopic sites.

One member of our group is responsible for a facility within the Molecular Biotechnology Center in Torino, aimed at the preparation of transgenic mice using recombinant ES cells. In routine work, it became necessary to have a rapid test to exclude the presence of additional copies of the *NEO* cassette in ES clones in which homologous recombination was successfully obtained. Here we describe a screening method using a rapid semi-quantitative real-time PCR, which was validated on ES clones with different *NEO* copies (0, 1, 2, > 2 copies), previously assessed by Southern blot.

From one of the projects involving the preparation of recombinant mice, we selected 45 genomic DNA

\* Correspondence: [alfredo.brusco@unito.it](mailto:alfredo.brusco@unito.it)

<sup>1</sup>Department of Genetics, Biology and Biochemistry, University of Torino, Torino, Italy

Full list of author information is available at the end of the article


extracted from ES clones that then underwent Southern blot screening. DNA extraction was performed using standard phenol-chloroform method [7]. Southern blot was performed using standard conditions for gel run, transfer and hybridisation. A *NEO* probe of 773 bp was used to evaluate the number of transgenic plasmid insertions.

As an alternative or complementary method to assess the *NEO* cassette copy number, we set up an assay based on quantitative real-time PCR (qPCR). The assay was performed with two protocols on an ABI 7500 Fast instrument (Applied Biosystems, Foster City, CA, USA); data were analyzed using the 7500 software. The two approaches were: (i) an MGB-based assay (MGB-assay), and (ii) a SYBR Green-based assay (SYBR-assay) (Applied Biosystems). Using the Primer Express software (Applied Biosystems) we designed specific PCR primers to amplify 62 bp of highly conserved sequences between two

different *NEO* cassette-containing plasmids PL451 and PL452 (<http://web.ncifcrf.gov/research/brb/recombineeringInformation.aspx>). The mouse *Rpp30* gene (63 bp, RefSeq NM\_019428.3) was used as a reference gene. This gene is orthologous to the human *RNaseP*, widely used as a copy number reference in qPCR assay. Real-time PCR conditions and primer sequences are reported in Figure 1.

In the MGB-assay we combined the two *NEO* and *Rpp30* assays in a duplex PCR including two internal Taqman-MGB probes (5'-FAM labelled for *NEO* and 5'-VIC labelled for *Rpp30*) (Figure 1). Each sample was consistently run in triplicate with a blank well to check for contaminations.

In the SYBR-assay the two reactions were run in separate wells, using a Fast SYBR green mix (Applied Biosystems). The efficiency of each assay was verified with a standard curve starting from 100 ng of mouse DNA, using

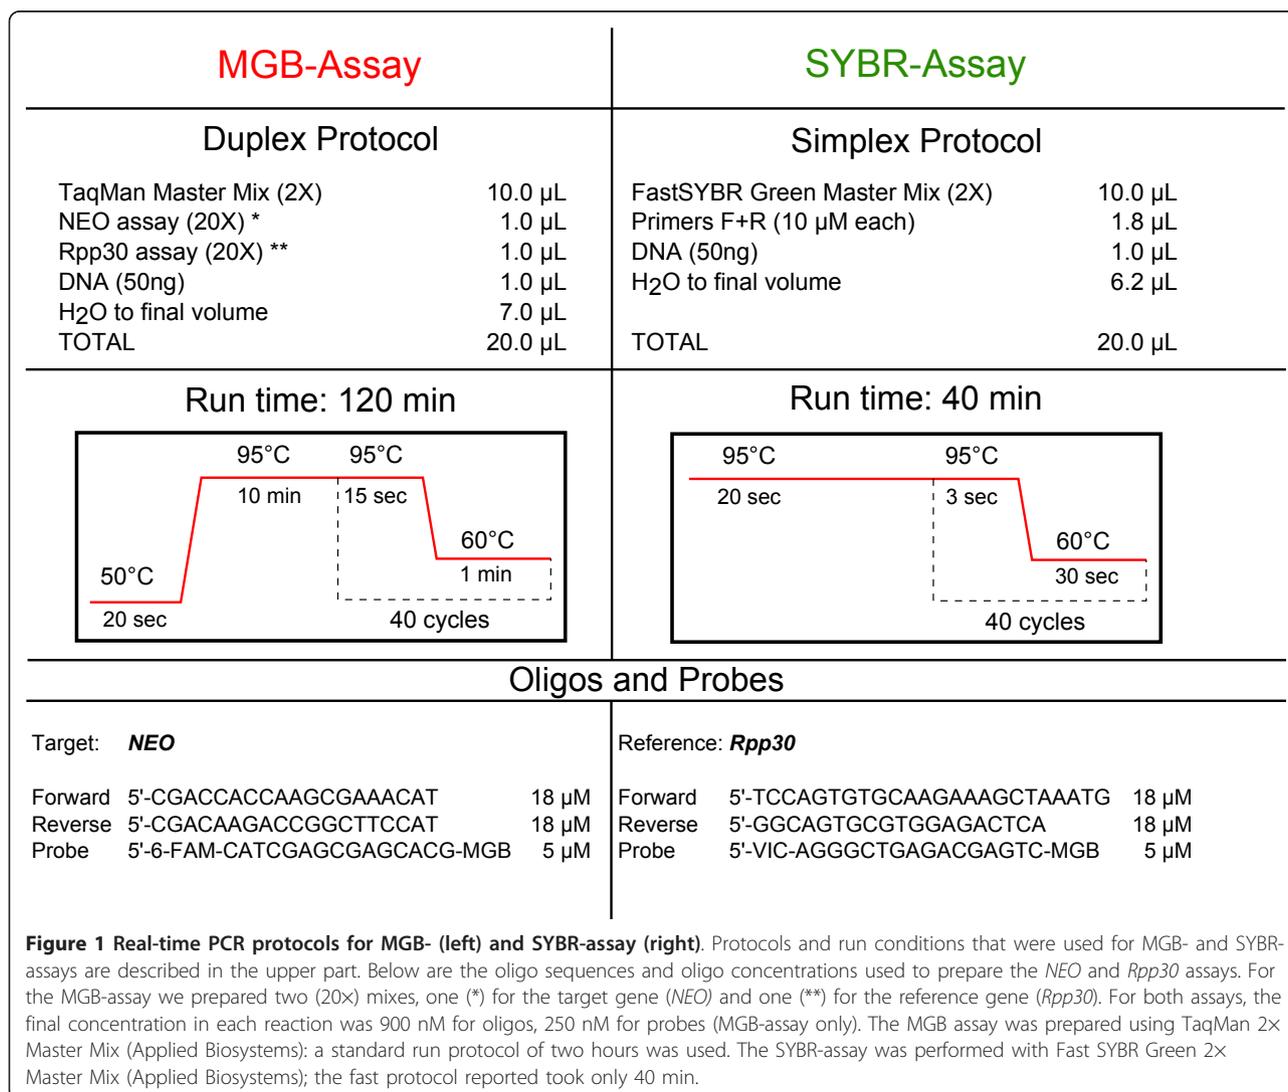



control DNA with two *NEO* copies, the value of *nNEO* was 2.2 for the MGB-assay and 2.4 for the SYBR-assay (Figure 2A).

The remaining 23 ES clones ( $\geq 2$  *NEO* copies) showed a variable number of *nNEO* from  $\sim 2$  to  $> 60$  (Figure 2B). Comparing results of the two qPCR assays for the same sample, we saw that the values of *nNEO* had a minimal variability. Although the *nNEO* number probably reflects the amount of cassettes, calculating their exact number was beyond our scope. Curiously, we found high copy-number insertions that reached up to 60; this could be explained by the presence of concatamers of the vector, rather than multiple insertions in the mouse genome.

Southern blot analysis has long been the reference method for the detection of *NEO* copy number in ES clones. However, this method requires large amounts of DNA samples, as well as being laborious, time-consuming, and sometimes difficult to interpret. Our experience in transgenic mouse model preparation has led to the conclusion that having an alternative method is highly favourable. We propose a semi-quantitative real-time PCR method, that only requires small amounts of DNA, and much less time to be performed (the Fast, SYBR-assay format takes under one hour). This method appears to be sensitive enough even for identification of single *NEO* insertions. Of the two assays tested, the MGB-assay is the least convenient, as it requires two specific and expensive fluorescently-labelled probes, and does not show any practical advantage over the SYBR-assay.

Approaches based on real-time PCR to validate ES positive clones have been previously described, using absolute quantification of *NEO*, or a relative quantification to detect deletion of the target gene [9,10]. Our method, based on a relative PCR quantification, can be easily reproduced in other laboratories using different technical platforms, and does not need the preparation of standards.

One possible drawback may be the genomic DNA quality/degradation that needs to be checked in case of non-reproducible data.

In conclusion, our real-time PCR assay to quantify *NEO* copy number is a valid alternative tool to Southern blot for the rapid screening of large numbers of ES cell clones during the production of knockout or knockin mouse models.

#### Acknowledgements

This work was supported by Telethon research grant GGP07110 to AB.

#### Author details

<sup>1</sup>Department of Genetics, Biology and Biochemistry, University of Torino, Torino, Italy. <sup>2</sup>S.C.D.U. Medical Genetics, A.O.U. San Giovanni Battista, Torino, Italy. <sup>3</sup>Molecular Biotechnology Center, Torino, Italy.

#### Authors' contributions

CM and EM carried out laboratory experiments, analyzed data and drafted the manuscript; ET analyzed data and revised the manuscript; AB and AB designed the experiments, analyzed data, drafted and revised the manuscript.

All authors read and approved the final manuscript.

#### Competing interests

The authors declare that they have no competing interests.

Received: 29 July 2011 Accepted: 28 October 2011

Published: 28 October 2011

#### References

1. Thomas KR, Deng C, Capecchi MR: High-fidelity gene targeting in embryonic stem cells by using sequence replacement vectors. *Mol Cell Biol* 1992, **12**:2919-2923.
2. Meier ID, Bernreuther C, Tilling T, Neidhardt J, Wong YW, Schulze C, Streichert T, Schachner M: Short DNA sequences inserted for gene targeting can accidentally interfere with off-target gene expression. *FASEB J* 2010, **24**:1714-1724.
3. Joyner A: *Gene targeting a practical approach* New York: Oxford University Press; 2000.
4. Olson EN, Arnold HH, Rigby PW, Wold BJ: Know your neighbors: three phenotypes in null mutants of the myogenic bHLH gene MRF4. *Cell* 1996, **85**:1-4.
5. Rijli FM, Dolle P, Fraulob V, LeMeur M, Chambon P: Insertion of a targeting construct in a *Hoxd-10* allele can influence the control of *Hoxd-9* expression. *Dev Dyn* 1994, **201**:366-377.
6. Pham CT, MacIvor DM, Hug BA, Heusel JW, Ley TJ: Long-range disruption of gene expression by a selectable marker cassette. *Proc Natl Acad Sci USA* 1996, **93**:13090-13095.
7. Sambrook J, Russell D: *Molecular Cloning: A Laboratory Manual* Cold Spring Harbor Laboratory Press; 2001.
8. Livak KJ, Schmittgen TD: Analysis of relative gene expression data using real-time quantitative PCR and the 2(-Delta Delta C(T)) Method. *Methods* 2001, **25**:402-408.
9. Valenzuela DM, Murphy AJ, Frenthewey D, Gale NW, Economides AN, Auerbach W, Poueymirou WT, Adams NC, Rojas J, Yassenchak J, et al: High-throughput engineering of the mouse genome coupled with high-resolution expression analysis. *Nat Biotechnol* 2003, **21**:652-659.
10. Coumoul X, Shukla V, Li C, Wang RH, Deng CX: Conditional knockdown of *Fgf2* in mice using Cre-LoxP induced RNA interference. *Nucleic Acids Res* 2005, **33**:e102.

doi:10.1186/1480-9222-13-10

Cite this article as: Mancini et al.: Gene-targeted embryonic stem cells: real-time PCR assay for estimation of the number of neomycin selection cassettes. *Biological Procedures Online* 2011 **13**:10.

**Submit your next manuscript to BioMed Central  
and take full advantage of:**

- Convenient online submission
- Thorough peer review
- No space constraints or color figure charges
- Immediate publication on acceptance
- Inclusion in PubMed, CAS, Scopus and Google Scholar
- Research which is freely available for redistribution

Submit your manuscript at  
www.biomedcentral.com/submit

